

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 07/13/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:24
INTERNAL STANDARD	VERIFIED	17:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:24
BLANK TEST	0.00	17:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	17:25
BLANK TEST	0.00	17:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:27
BLANK TEST	0.00	17:28

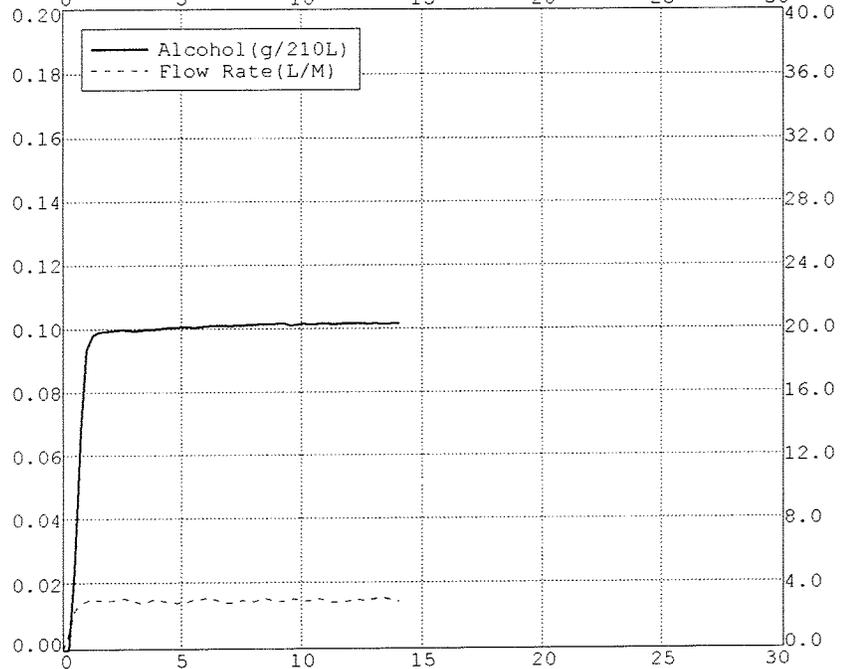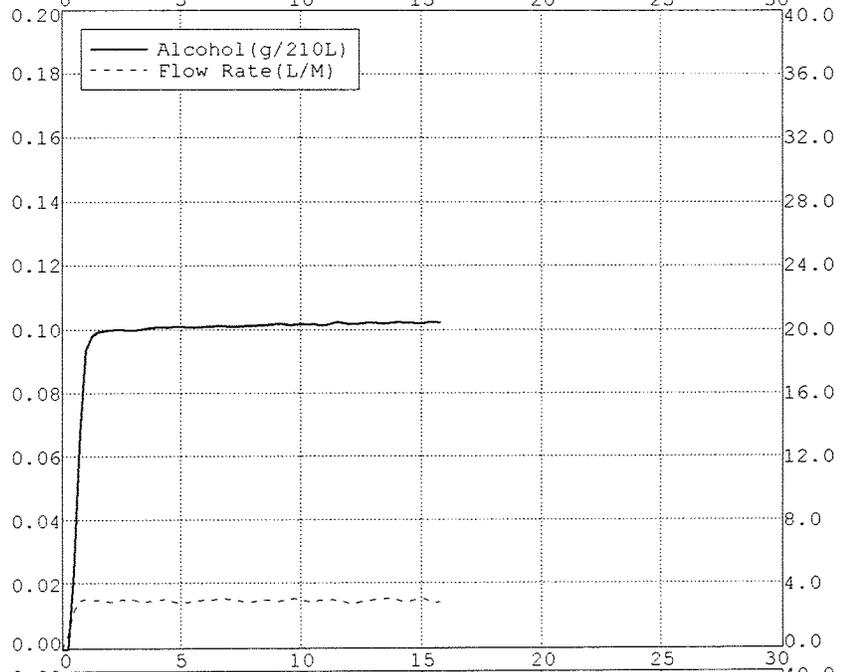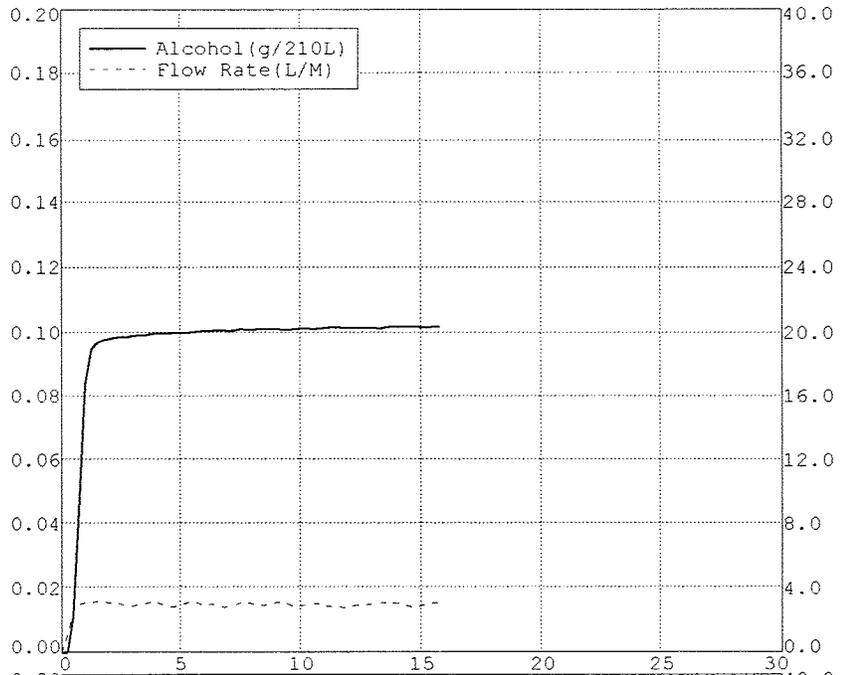

SGS *RJ Bartlett* WCO #162
 07-13-15