

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 07/19/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:01
INTERNAL STANDARD	VERIFIED	06:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:01
BLANK TEST	0.00	06:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:03
BLANK TEST	0.00	06:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:04
BLANK TEST	0.00	06:05

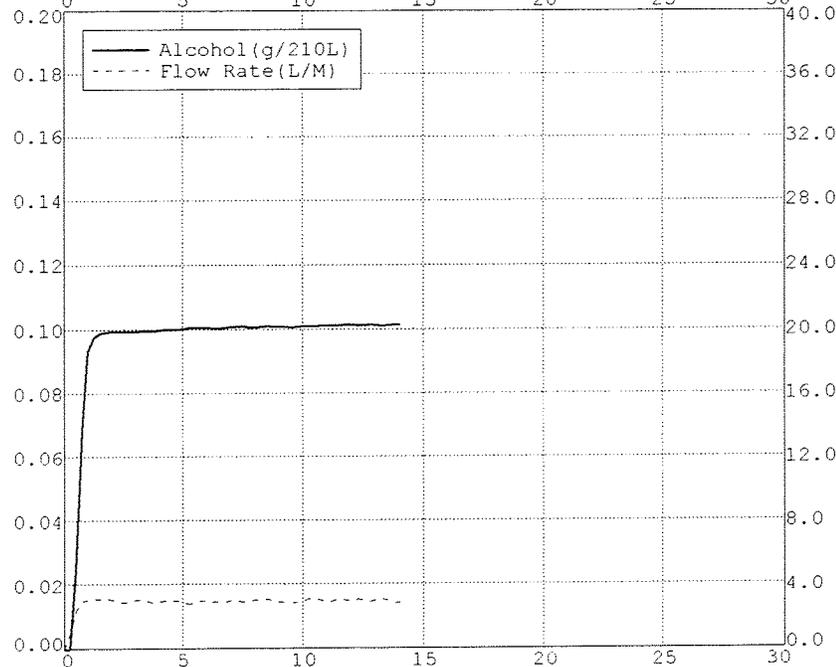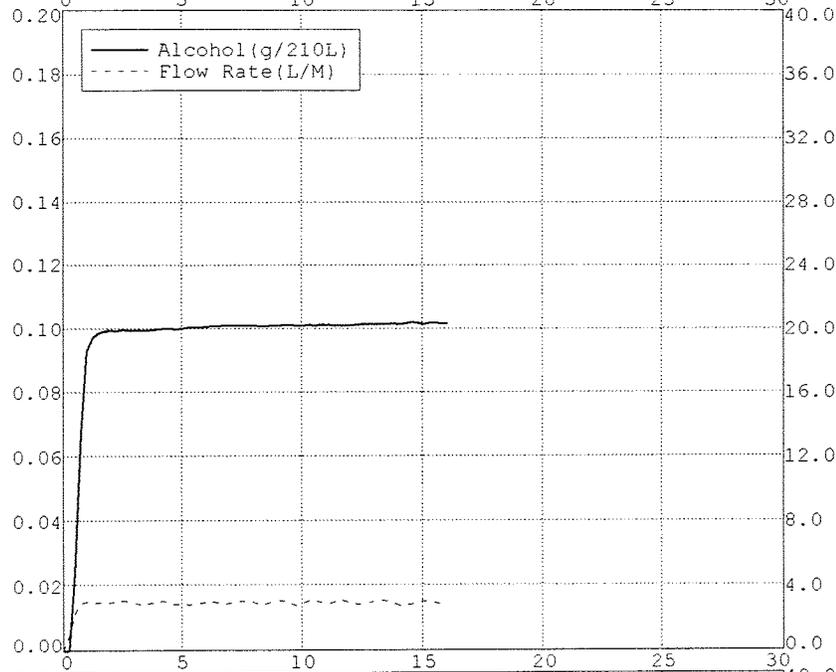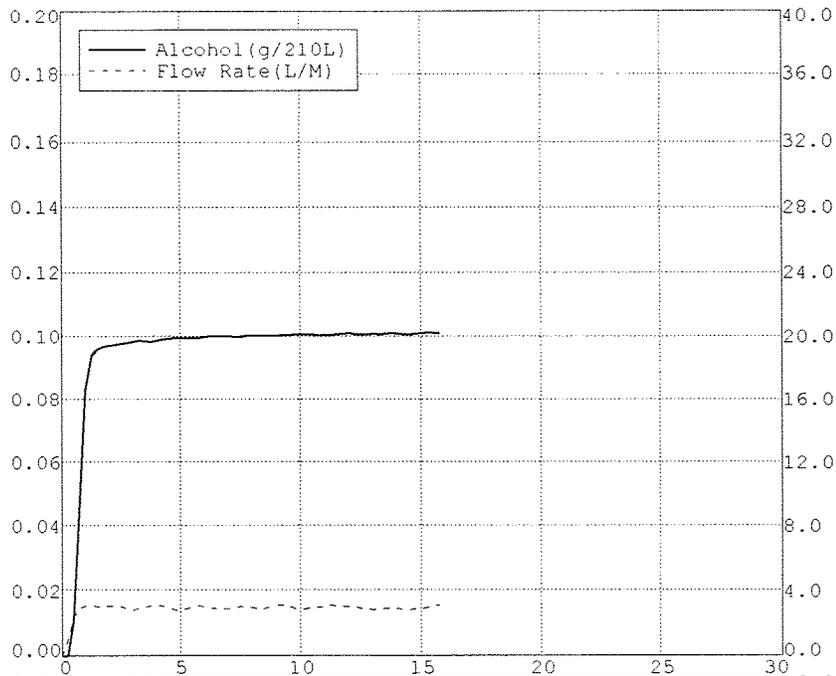

565 RLB Bartlett W&S #162

07-18-15