

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/25/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:08
INTERNAL STANDARD	VERIFIED	01:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:09
BLANK TEST	0.00	01:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:10
BLANK TEST	0.00	01:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:11
BLANK TEST	0.00	01:12

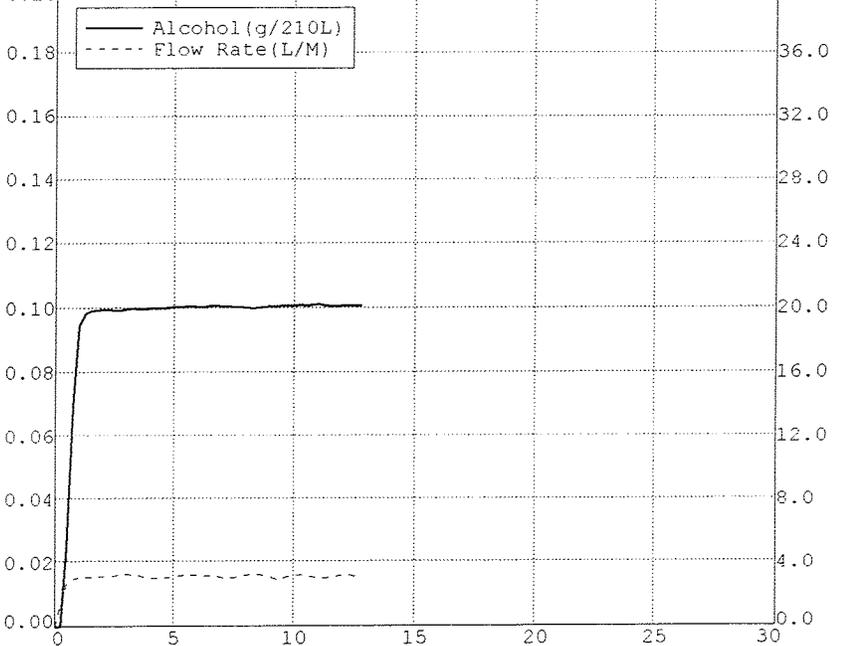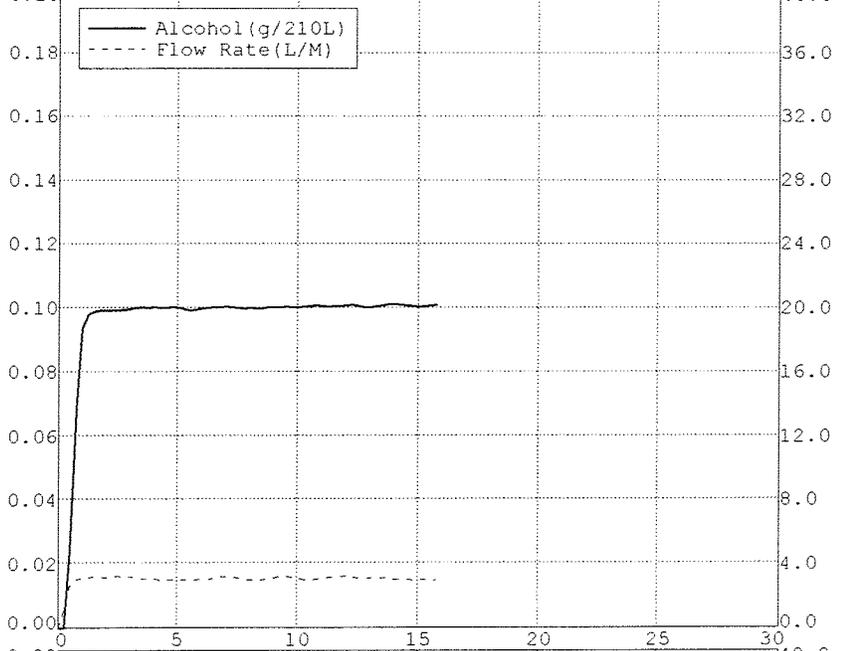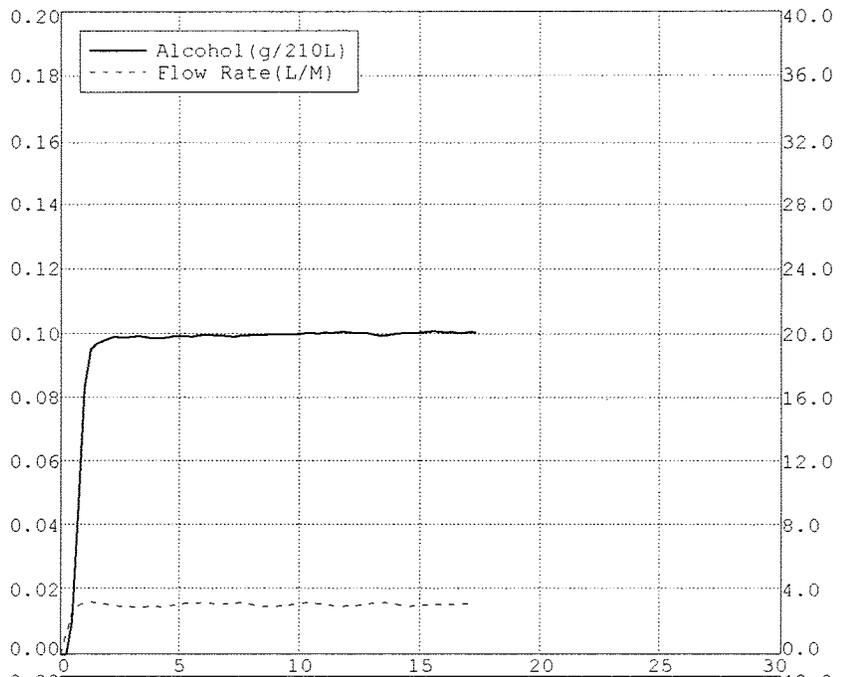

505 RJB Bartlett WLSO #102
08-25-15