

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/17/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:09
INTERNAL STANDARD	VERIFIED	06:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:10
BLANK TEST	0.00	06:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:11
BLANK TEST	0.00	06:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:12
BLANK TEST	0.00	06:13

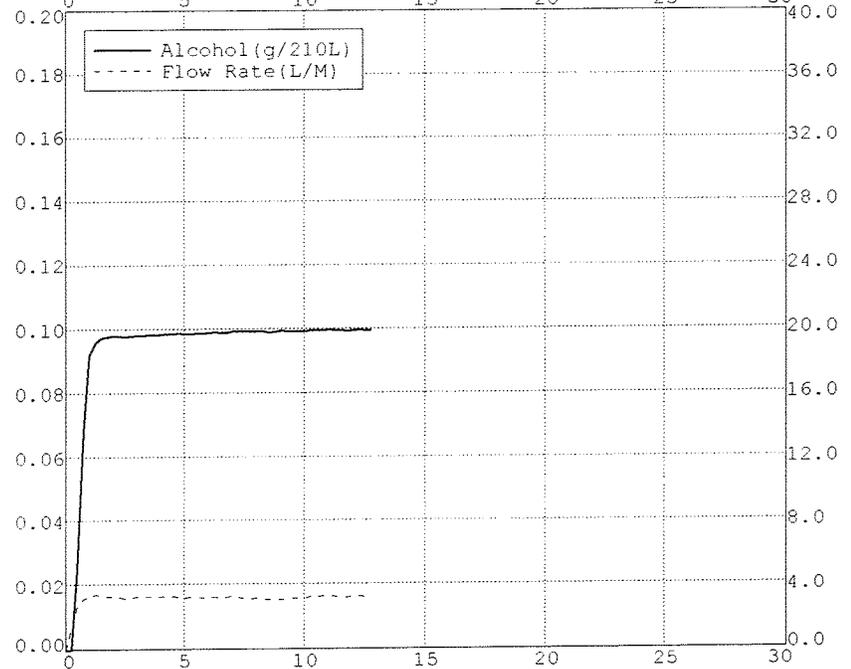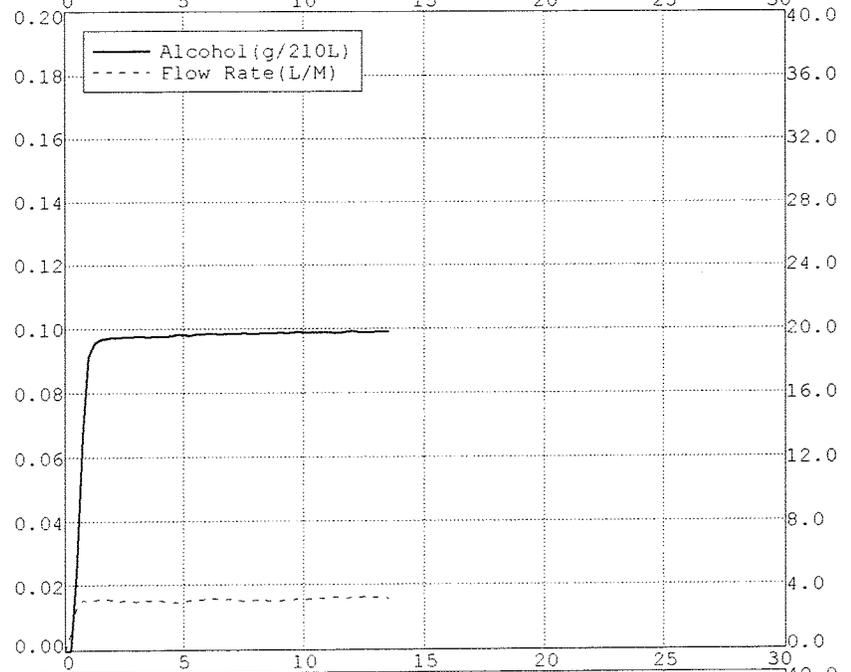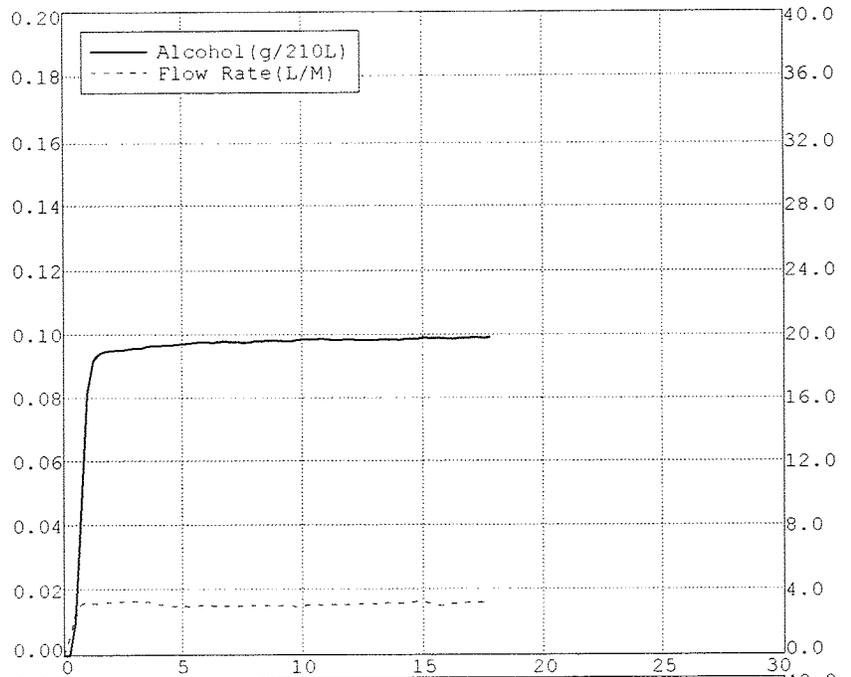

Sus Rly Bartlett waso #162
09-17-15