

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/22/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:18
INTERNAL STANDARD	VERIFIED	05:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:18
BLANK TEST	0.00	05:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	05:20
BLANK TEST	0.00	05:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:21
BLANK TEST	0.00	05:22

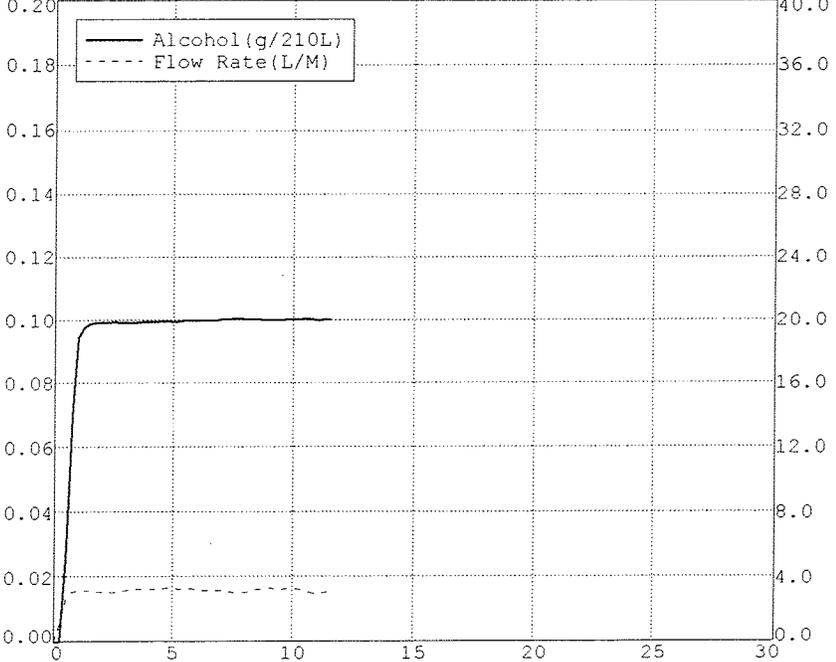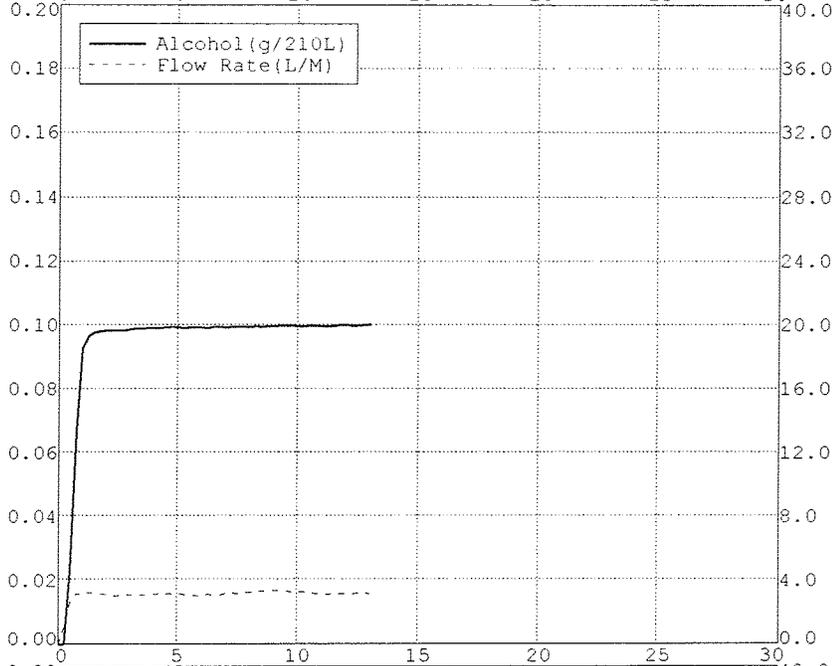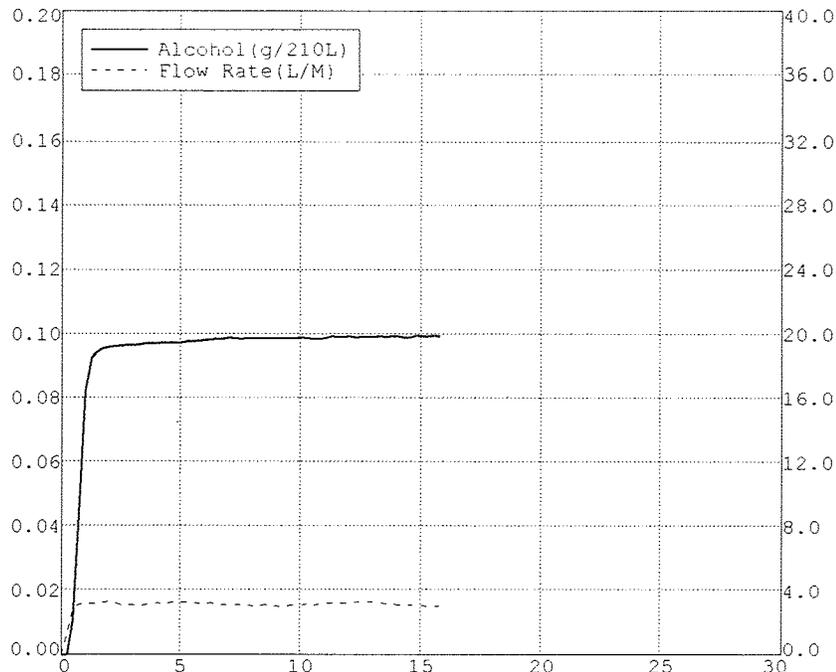

SCS *Ralph J Bartlett*
WC SO #162 09-22-15