

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 10/06/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:16
INTERNAL STANDARD	VERIFIED	03:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:17
BLANK TEST	0.00	03:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	03:18
BLANK TEST	0.00	03:19
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	03:19
BLANK TEST	0.00	03:20

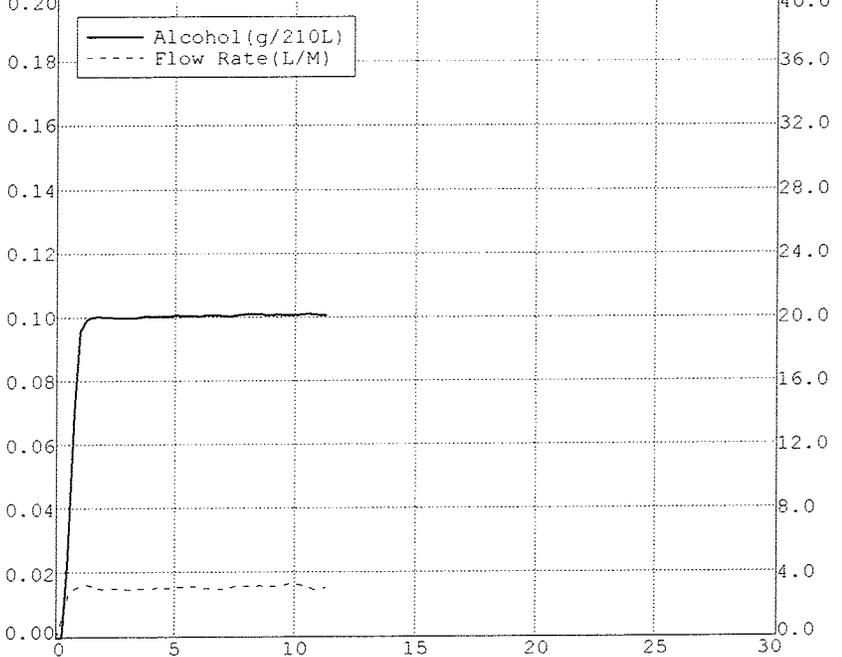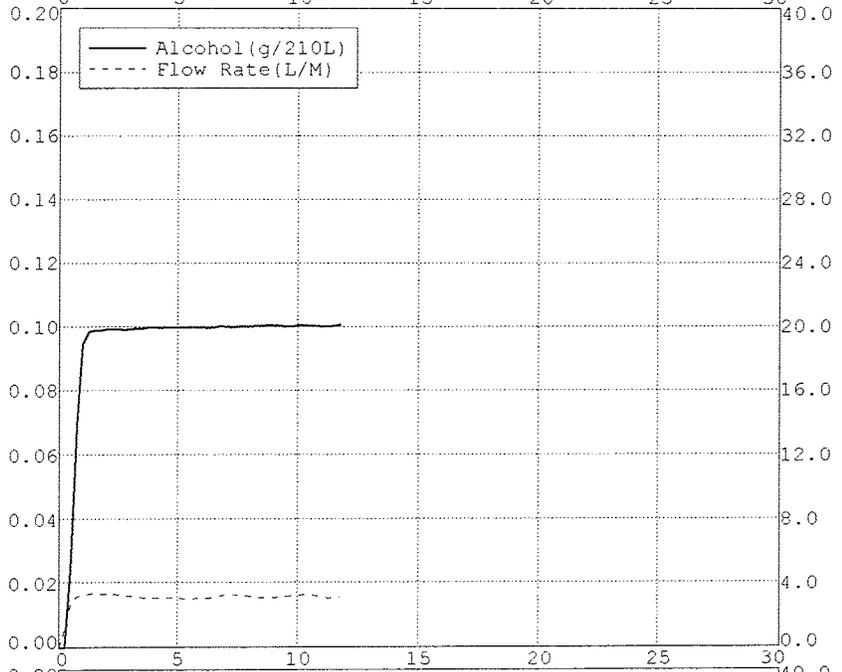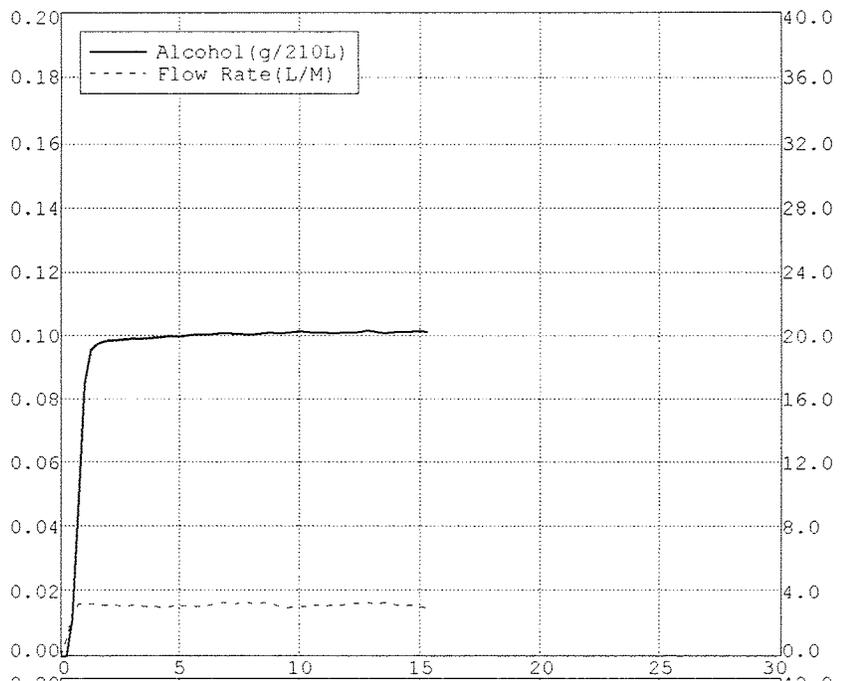

SG Bartlett 10-06-15
 WC 10 #162