

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/25/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:07
INTERNAL STANDARD	VERIFIED	06:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:07
BLANK TEST	0.00	06:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:09
BLANK TEST	0.00	06:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:10
BLANK TEST	0.00	06:11

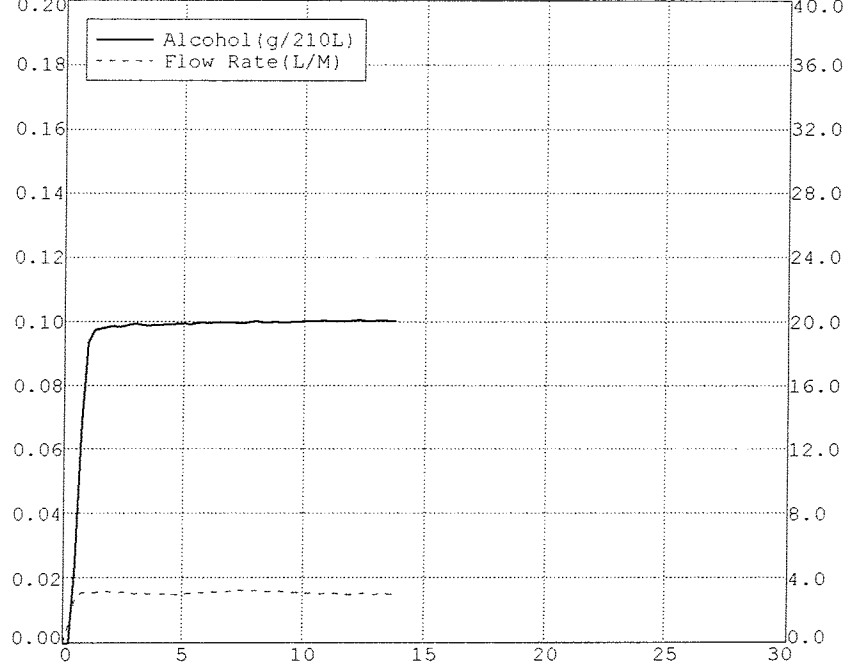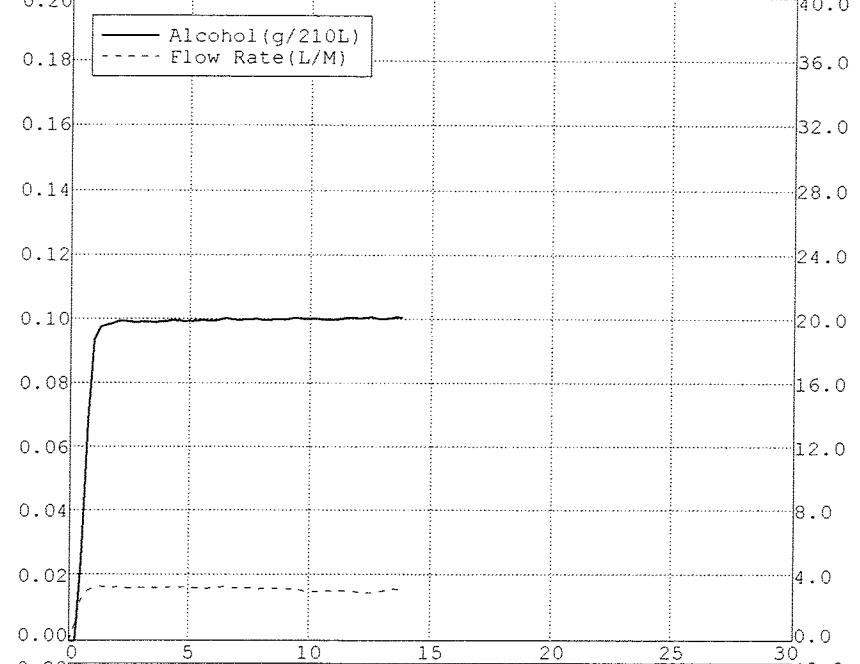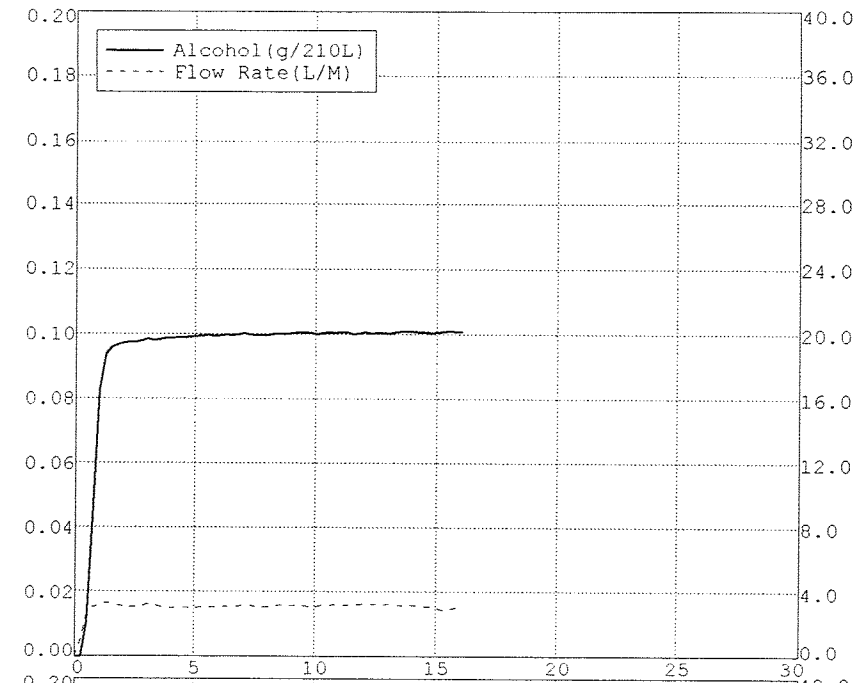

SGP RJB / Bartlett waso #162
10-25-15