

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/09/2015

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:43
INTERNAL STANDARD	VERIFIED	07:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:43
BLANK TEST	0.00	07:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:44
BLANK TEST	0.00	07:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:45
BLANK TEST	0.00	07:46

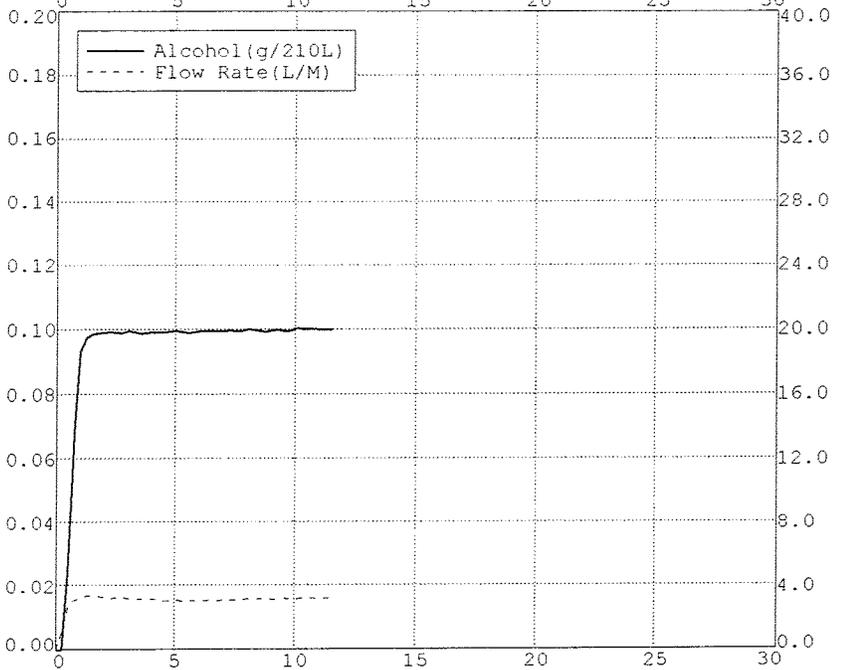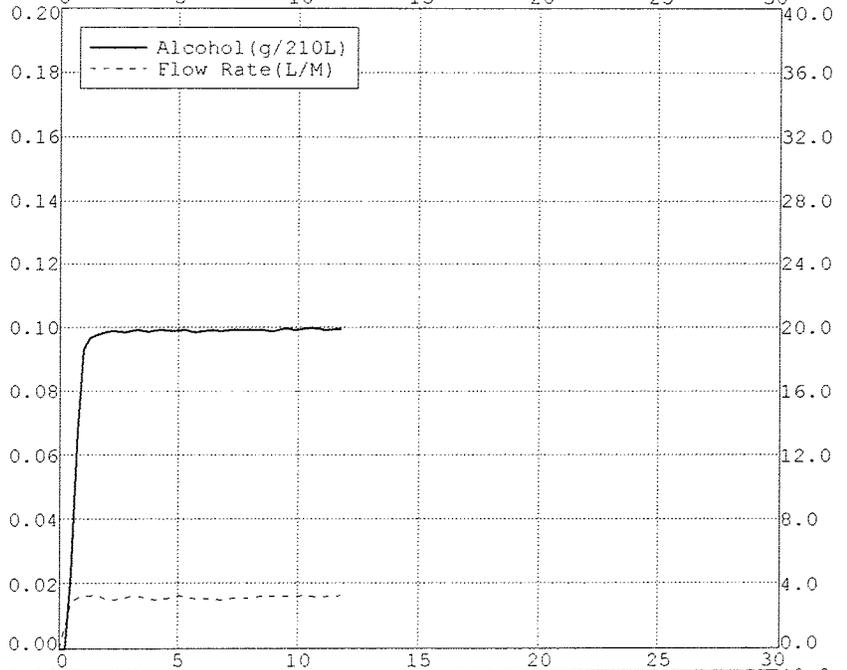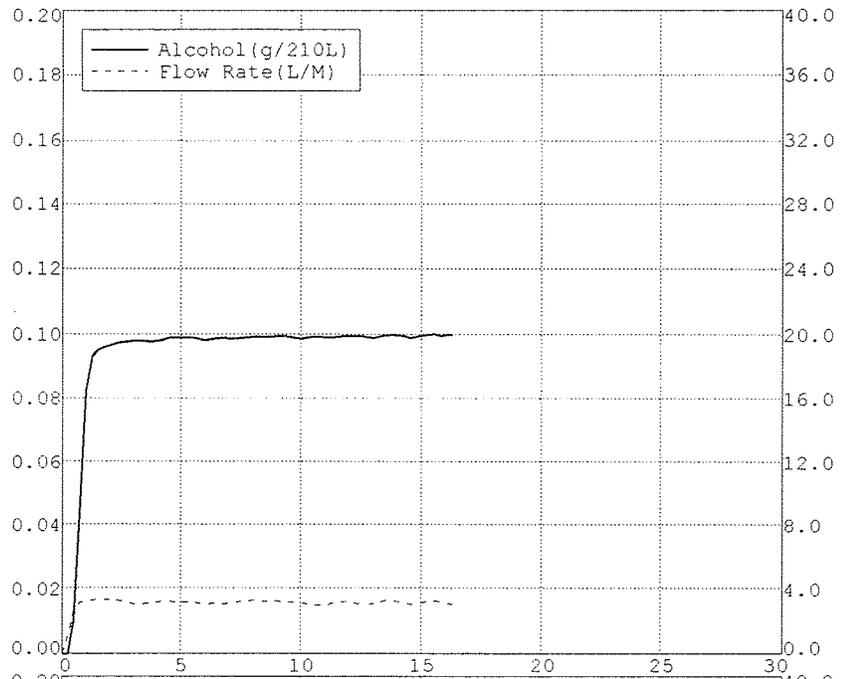

Charles B. Geisler #248 11/09/15