

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/15/2015

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15180

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 08:30 |
| INTERNAL STANDARD       | VERIFIED | 08:30 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 08:30 |
| BLANK TEST              | 0.00     | 08:31 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 08:32 |
| BLANK TEST              | 0.00     | 08:33 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 08:33 |
| BLANK TEST              | 0.00     | 08:34 |

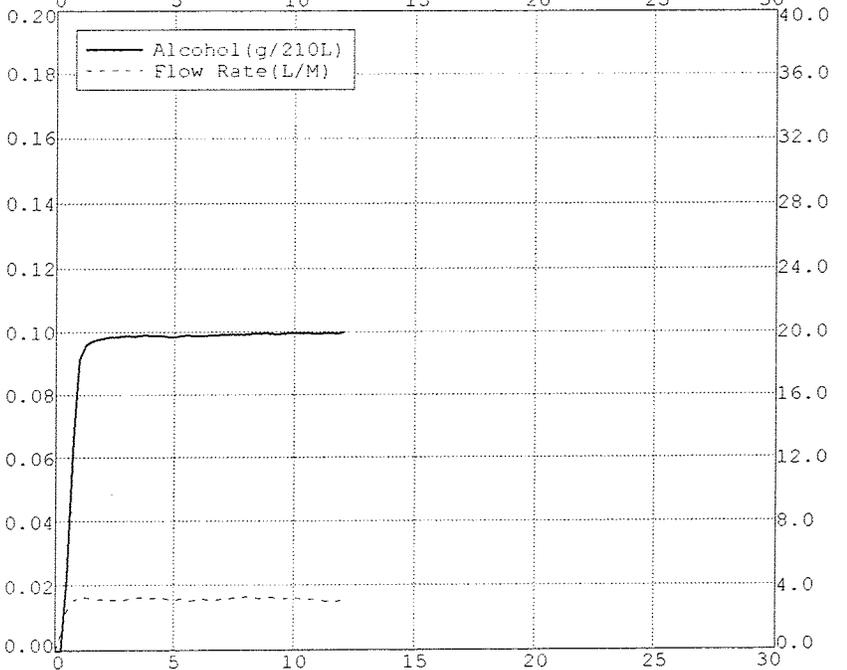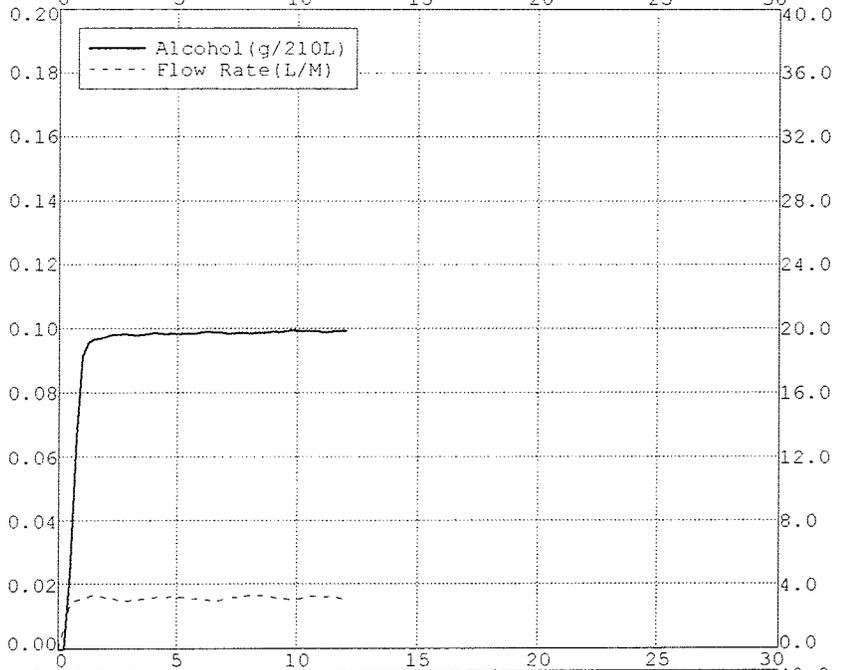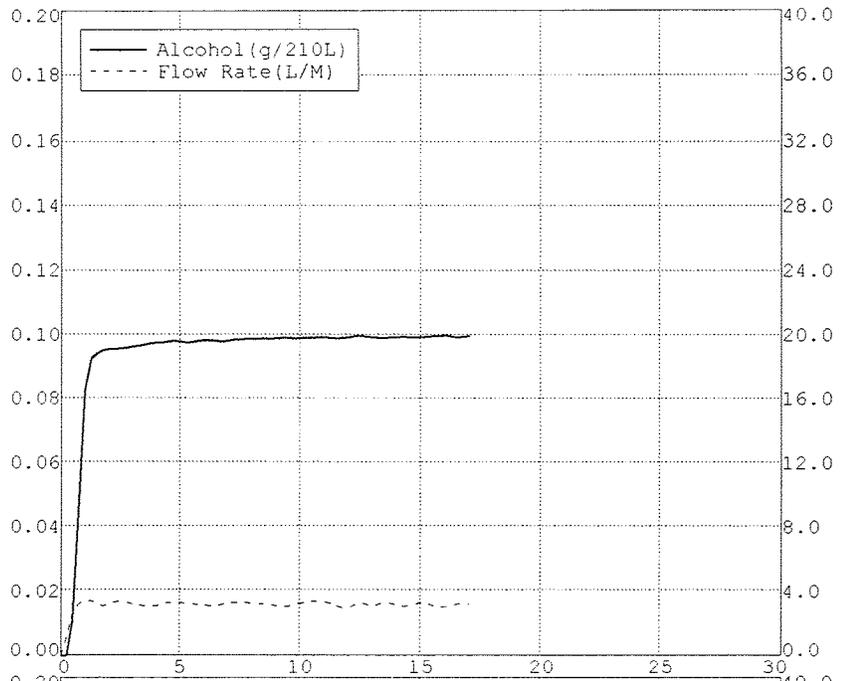

*Charles B. Geisler* #248 11/15/15  
0835