

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/23/2015

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:12
INTERNAL STANDARD	VERIFIED	13:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:13
BLANK TEST	0.00	13:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:14
BLANK TEST	0.00	13:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:15
BLANK TEST	0.00	13:16

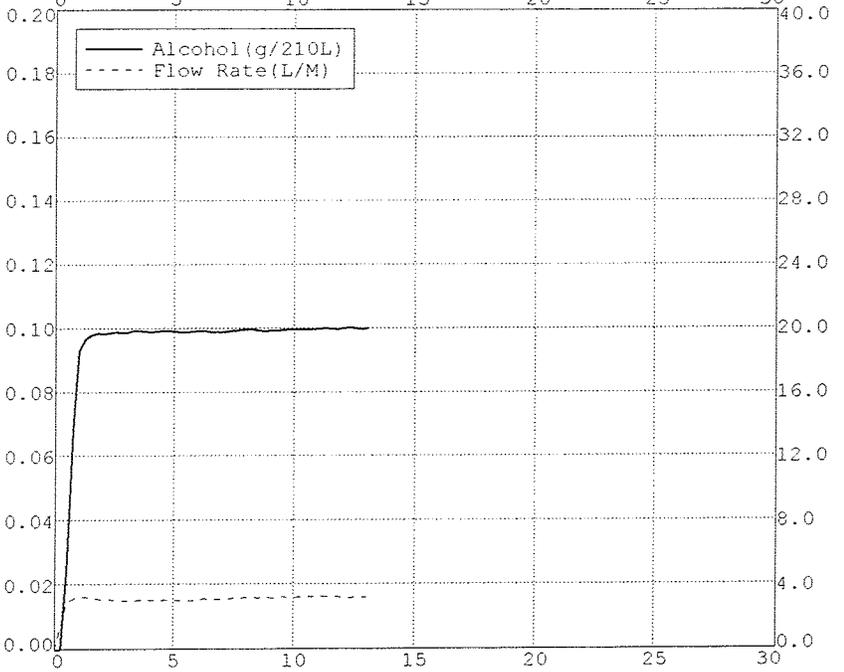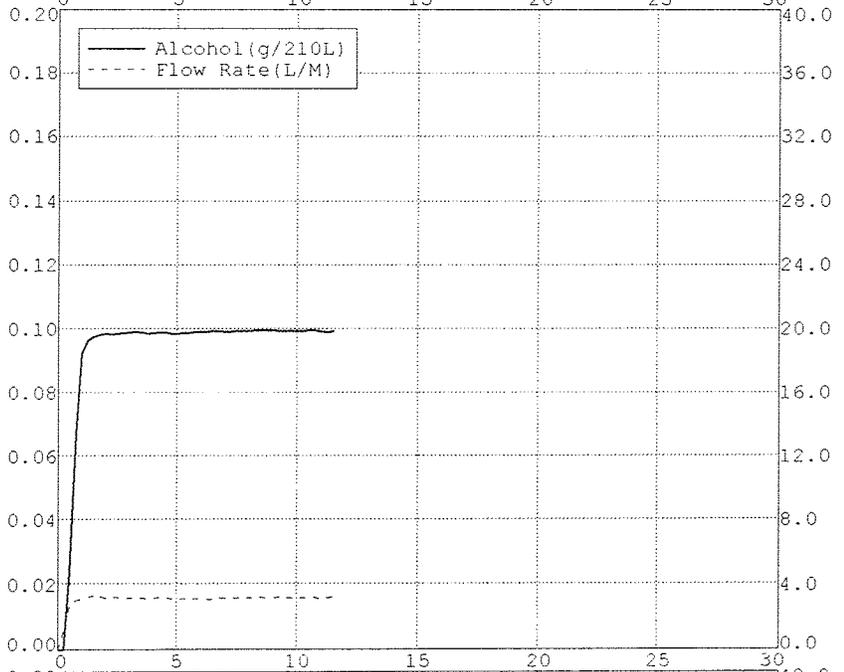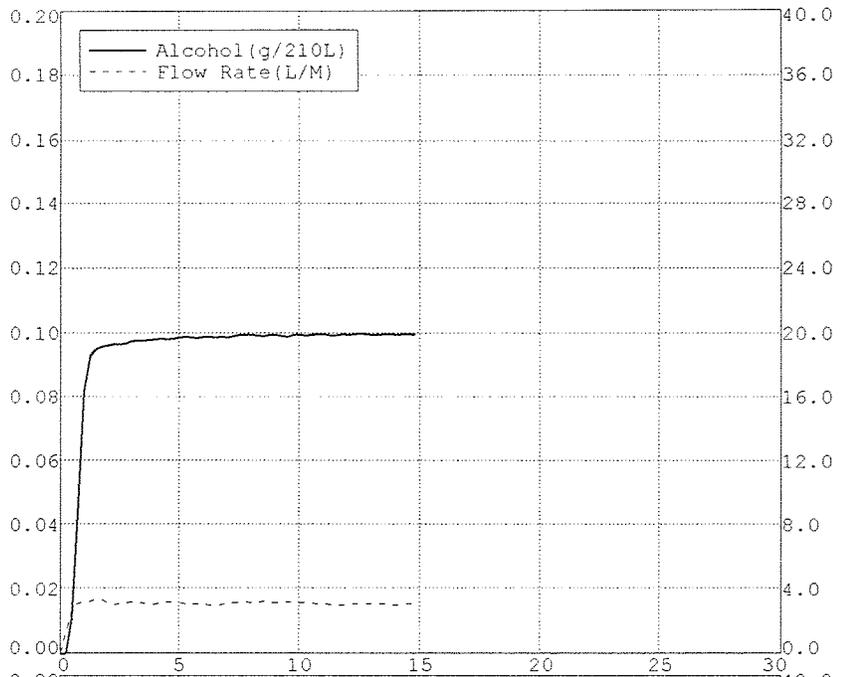

*Handwritten signature and notes:*  
#211 11/23/15  
1317 11/23