

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 12/01/2015

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:16
INTERNAL STANDARD	VERIFIED	03:16
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:16
BLANK TEST	0.00	03:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:18
BLANK TEST	0.00	03:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:19
BLANK TEST	0.00	03:20

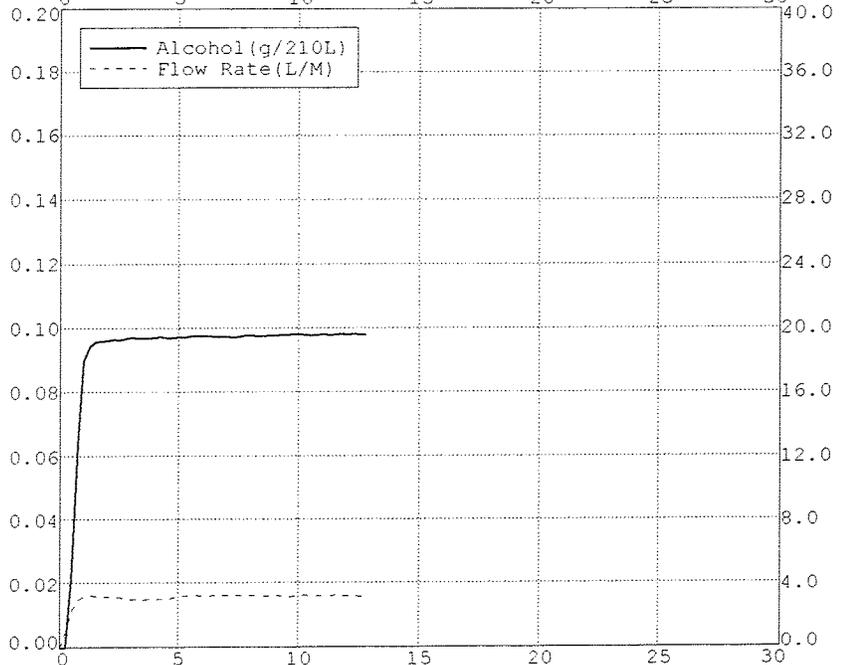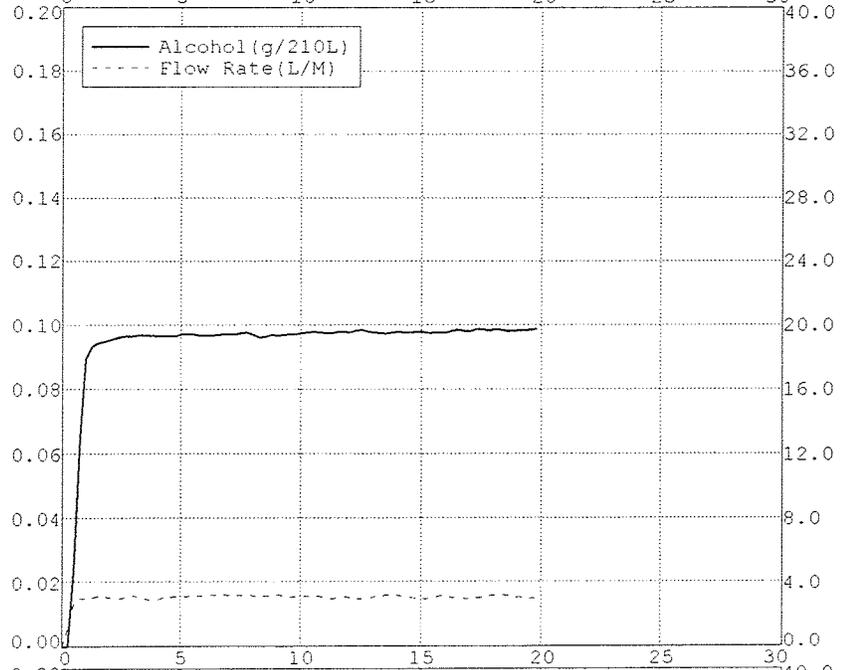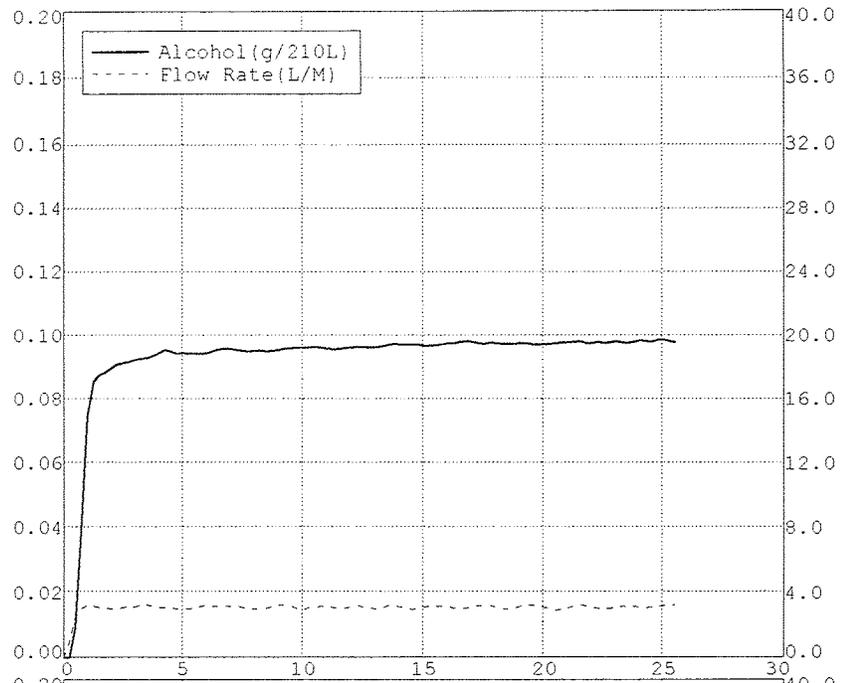

See Rly Results we-so #162

12-01-15