

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 12/09/2015

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:18
INTERNAL STANDARD	VERIFIED	23:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:19
BLANK TEST	0.00	23:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:20
BLANK TEST	0.00	23:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:21
BLANK TEST	0.00	23:22

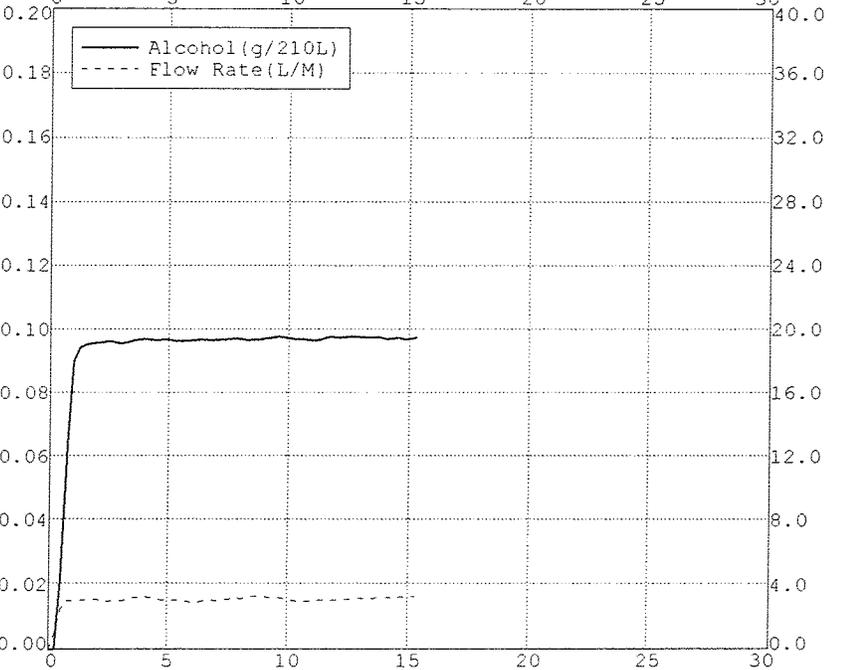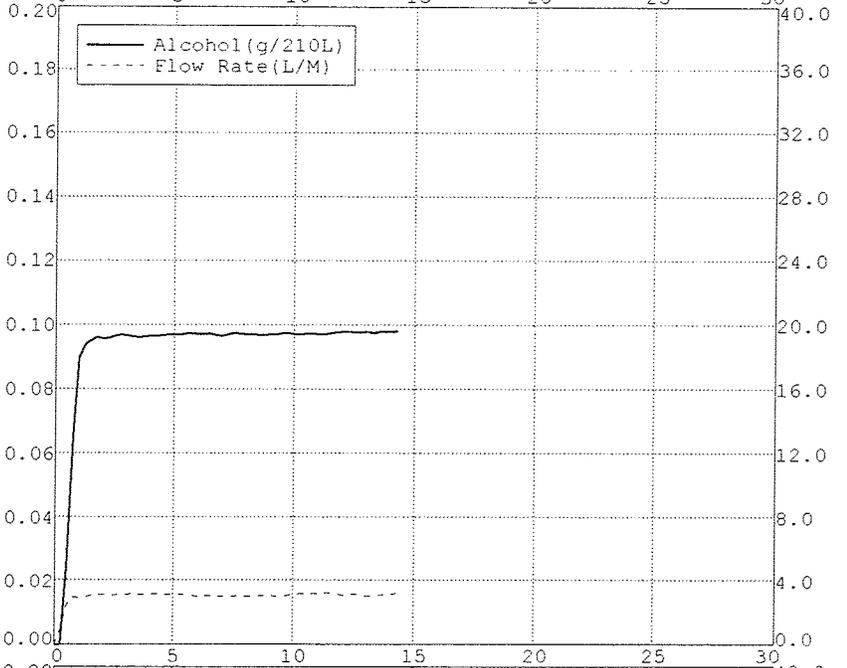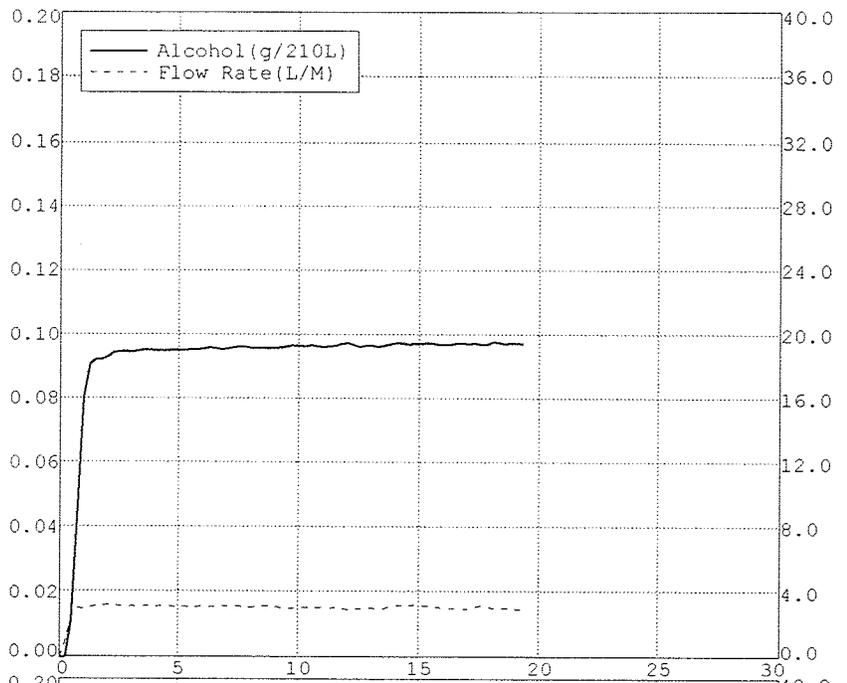

*SGT RJP* *Ritter* *WOSU #162*  
12/9/15