

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 12/29/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:13
INTERNAL STANDARD	VERIFIED	06:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:14
BLANK TEST	0.00	06:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:15
BLANK TEST	0.00	06:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:16
BLANK TEST	0.00	06:17

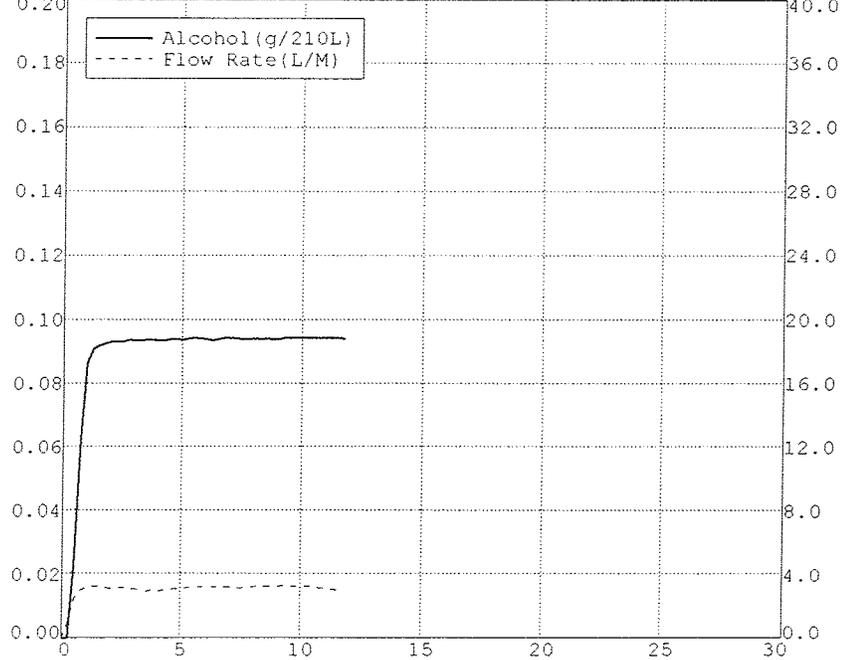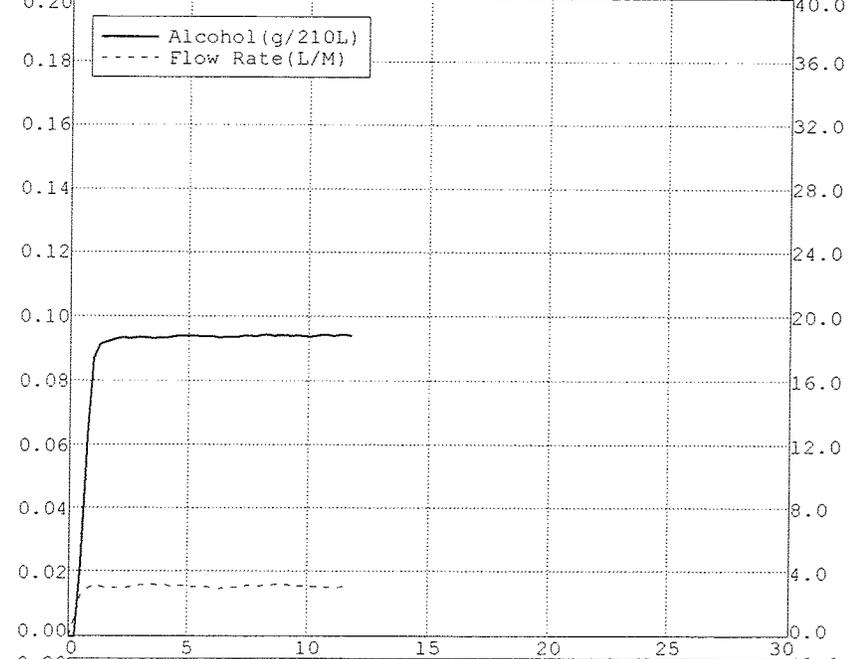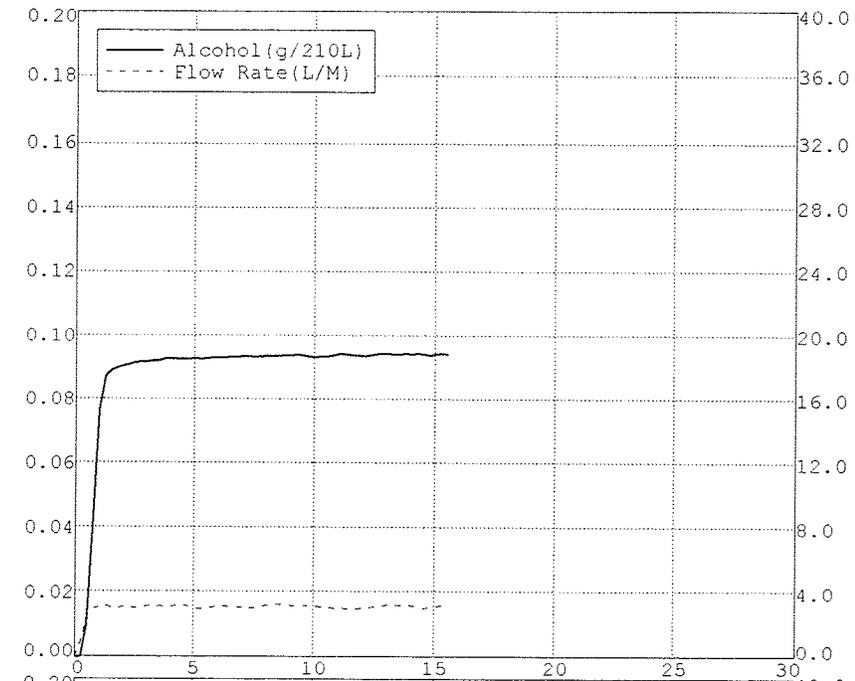

Sgt Ralph J Bartlett WOSO #162
 12/29/15