

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 01/19/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14230

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 00:45 |
| INTERNAL STANDARD | VERIFIED | 00:45 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 00:45 |
| BLANK TEST | 0.00 | 00:46 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 00:46 |
| BLANK TEST | 0.00 | 00:47 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 00:47 |
| BLANK TEST | 0.00 | 00:48 |

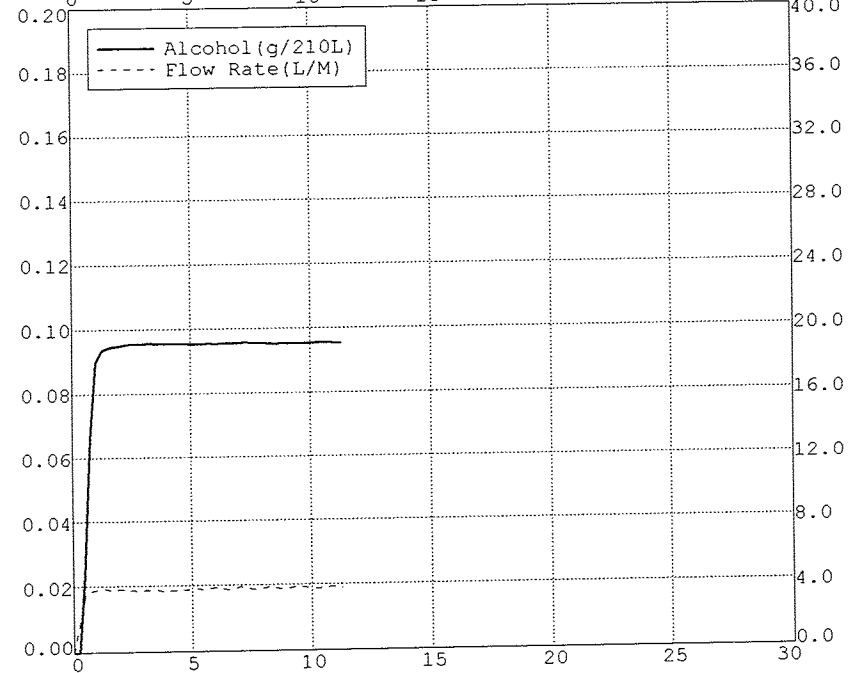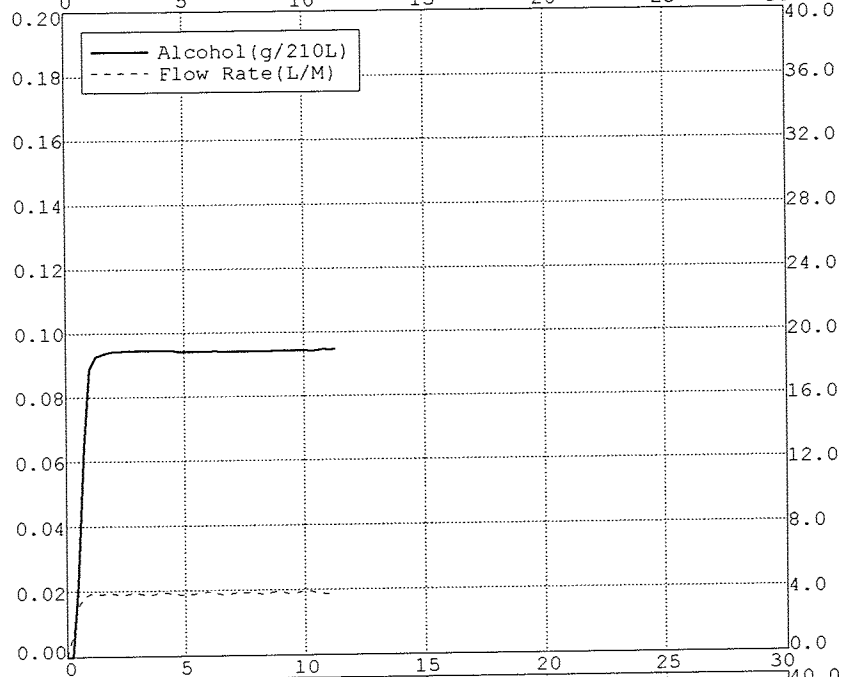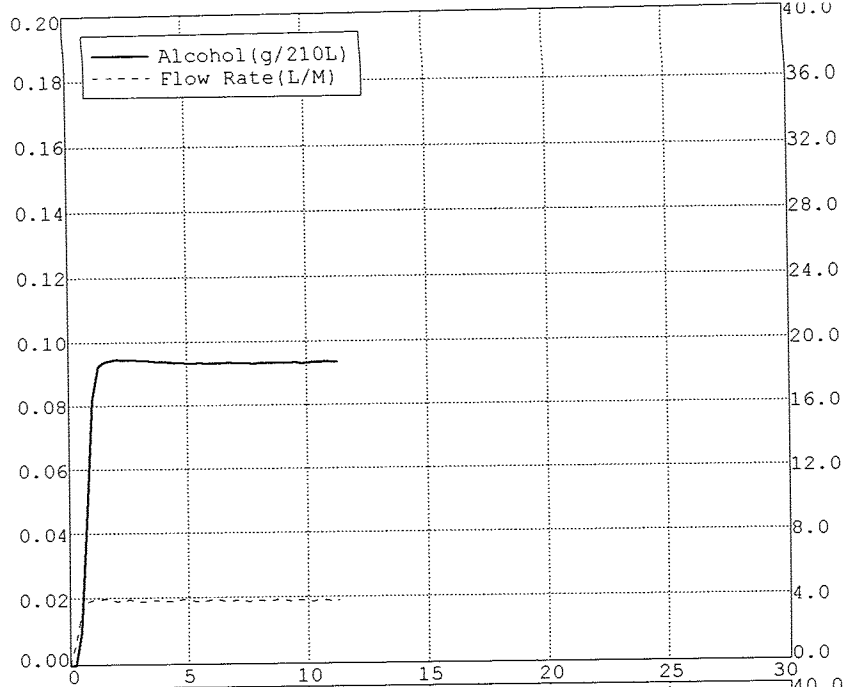

SGT R.J. Bartlett WESO #162
 01-19-15