

SOLUTION CHANGE




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/02/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15070

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 02:06 |
| INTERNAL STANDARD | VERIFIED | 02:07 |
| REFERENCE STANDARD TEMP | 33.98c | |
| REFERENCE STANDARD | 0.09 | 02:07 |
| BLANK TEST | 0.00 | 02:08 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 02:08 |
| BLANK TEST | 0.00 | 02:09 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 02:09 |
| BLANK TEST | 0.00 | 02:10 |

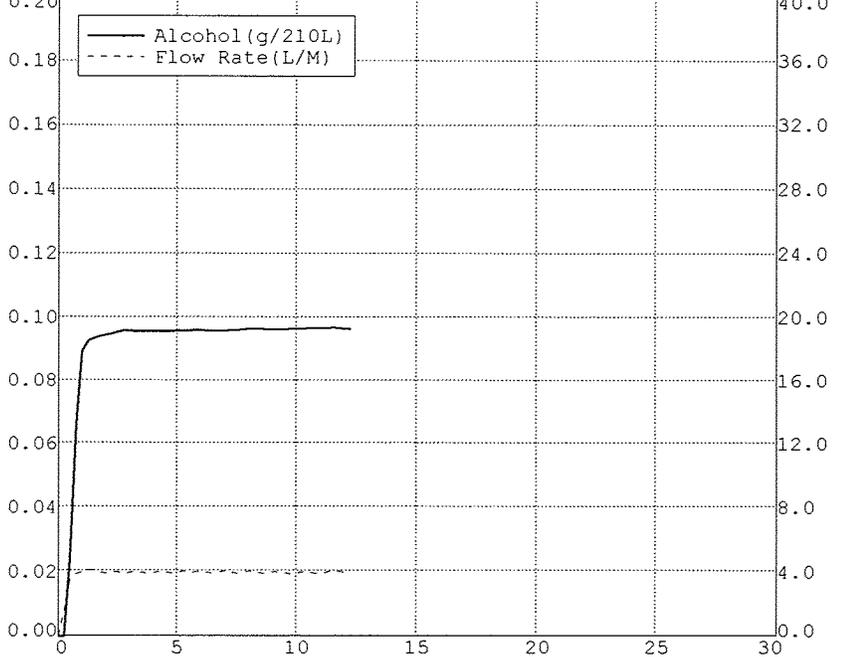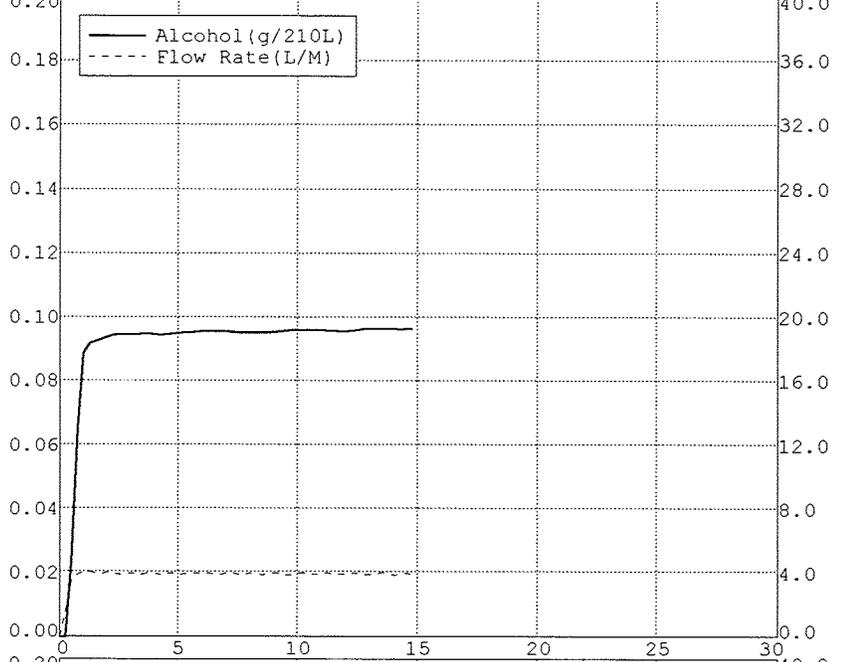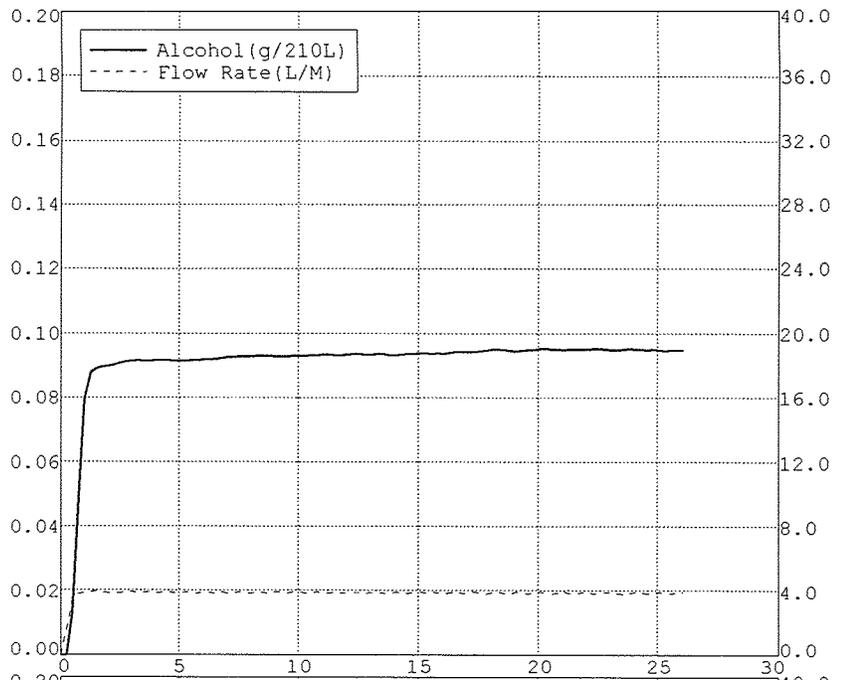

Sus Ralph Bartlett WCSO
#162
06-02-15