

SUPERVISOR TEST


WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/13/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:14
INTERNAL STANDARD	VERIFIED	18:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:14
BLANK TEST	0.00	18:15
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18

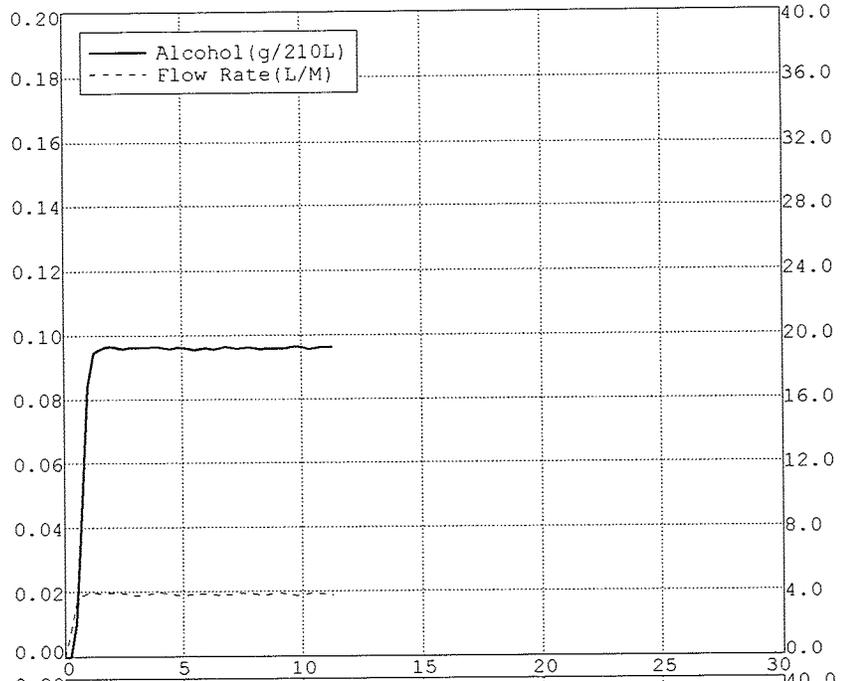

SGT R. J. Bartlett WSO #162
07-13-15