

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 11/15/2015

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:26
INTERNAL STANDARD	VERIFIED	10:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:27
BLANK TEST	0.00	10:28
REFERENCE STANDARD TEMP	34.04c	
REFERENCE STANDARD	0.09	10:28
BLANK TEST	0.00	10:29
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	10:29
BLANK TEST	0.00	10:30

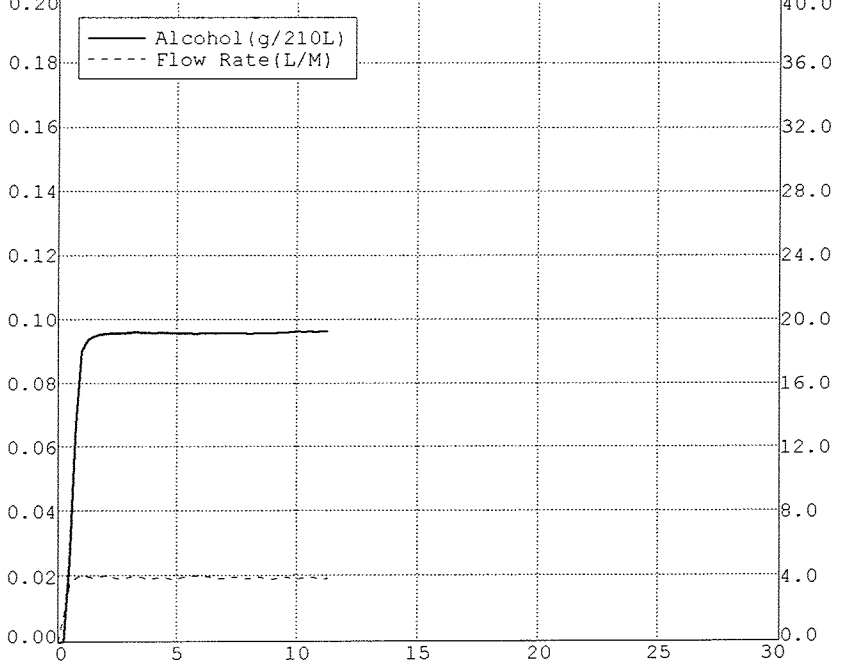

Handwritten signature and notes:
 #241 11/15/15 1032