

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/23/2015

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:49
INTERNAL STANDARD	VERIFIED	12:49
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	12:49
BLANK TEST	0.00	12:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	12:50
BLANK TEST	0.00	12:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:52
BLANK TEST	0.00	12:53

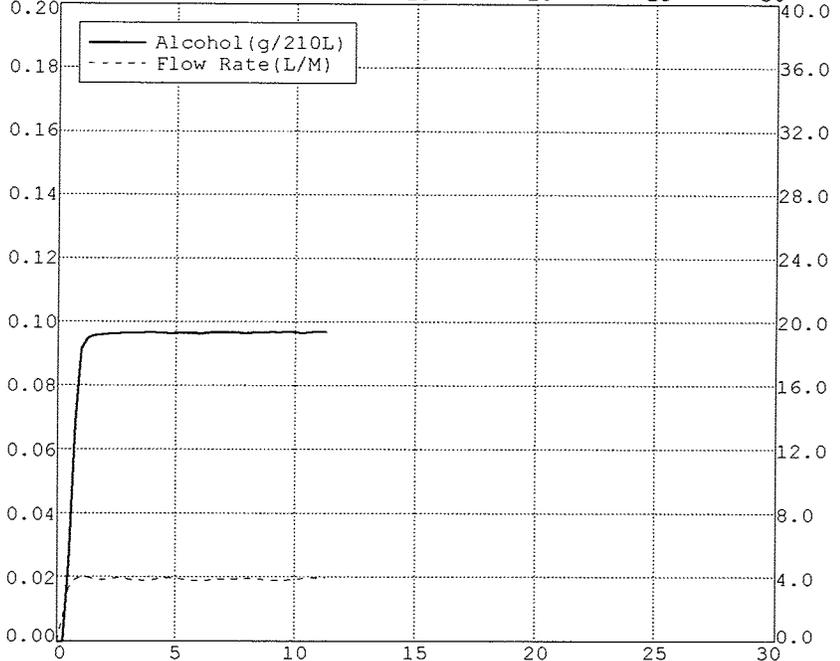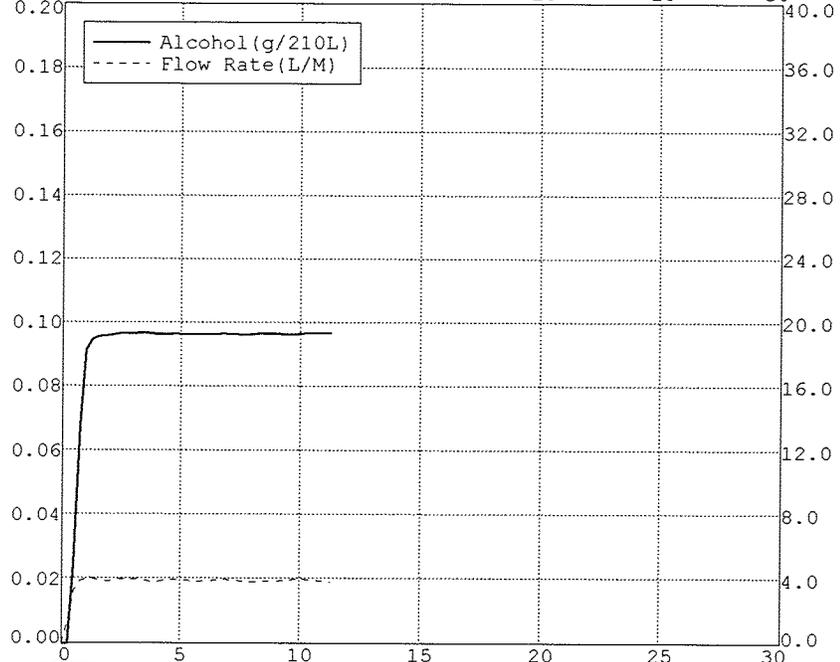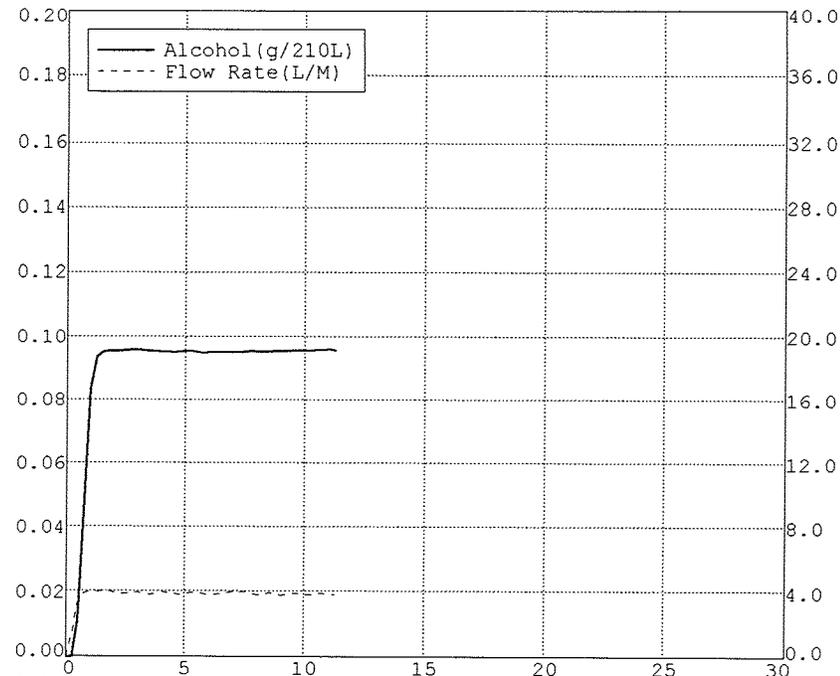

*Handwritten signature: C. B. Geisler #248 11/23/15*  
1254