

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/12/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:40
INTERNAL STANDARD	VERIFIED	01:40
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:41
BLANK TEST	0.00	01:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:42
BLANK TEST	0.00	01:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:43
BLANK TEST	0.00	01:44

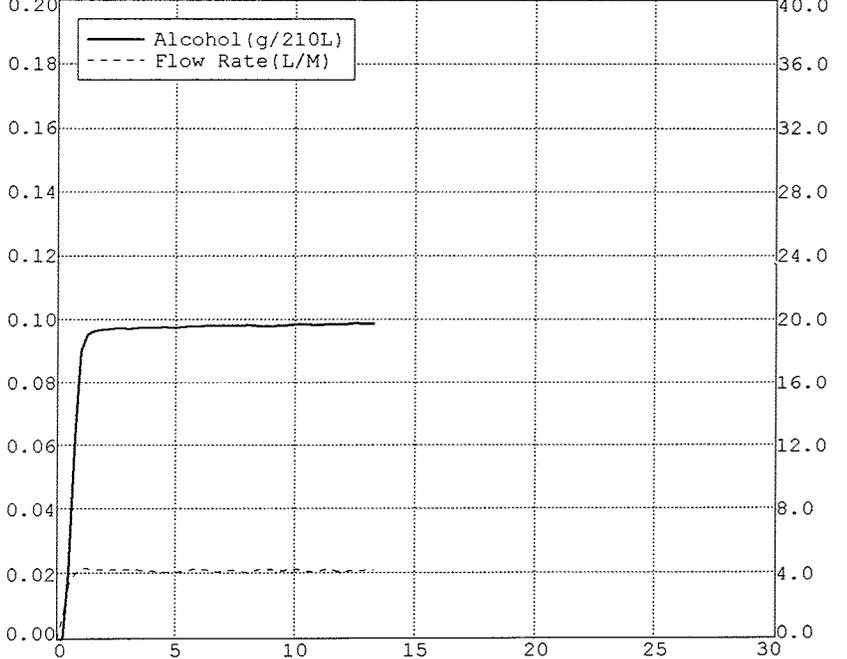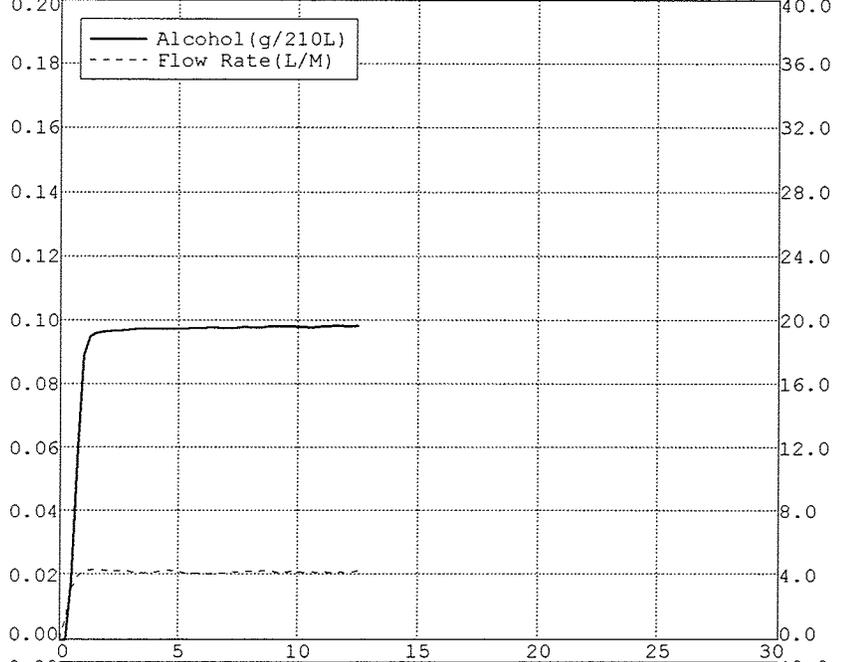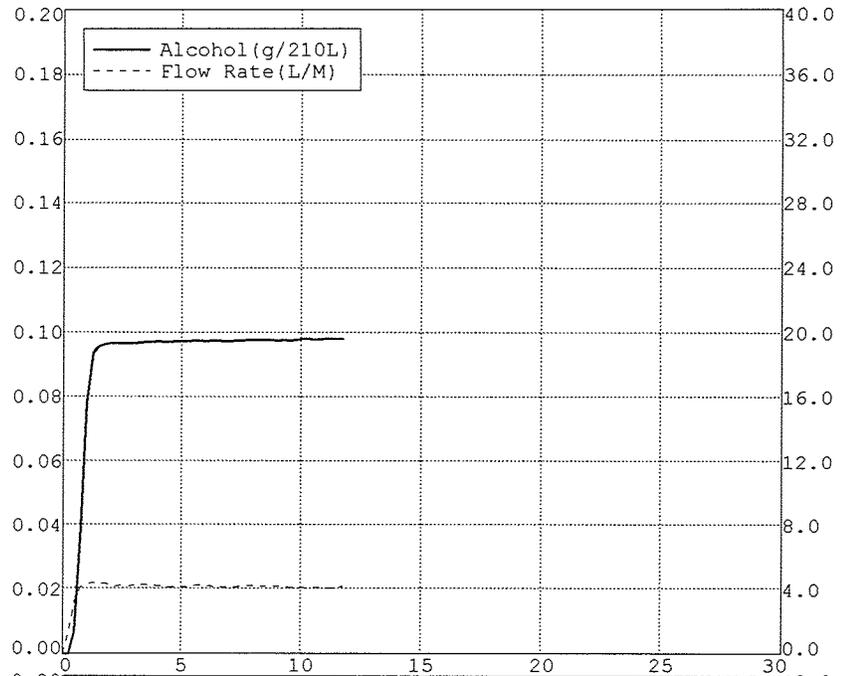

SGS *RJ Bartlett*

WCSO #102 01-12-16