

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/18/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:23
INTERNAL STANDARD	VERIFIED	01:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:26
BLANK TEST	0.00	01:27

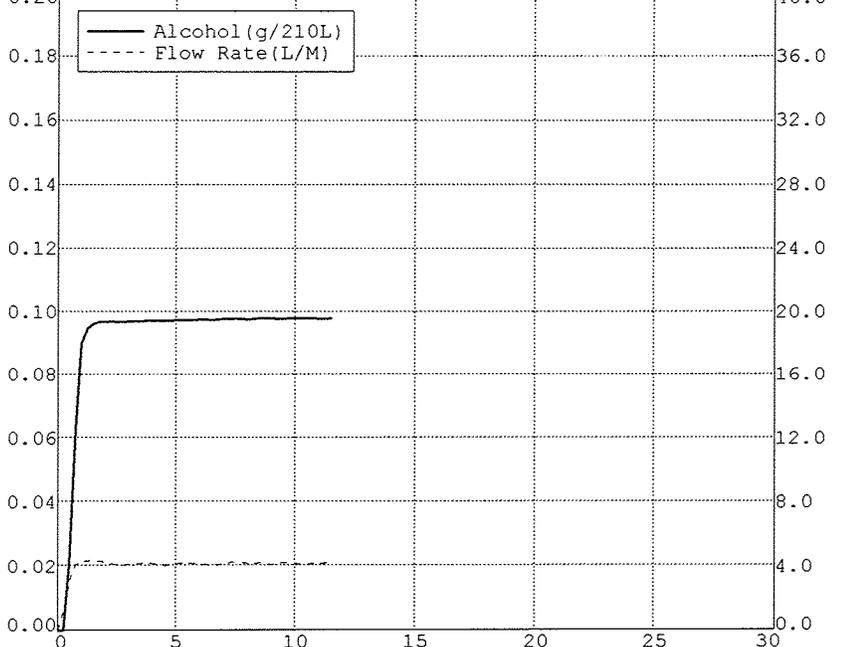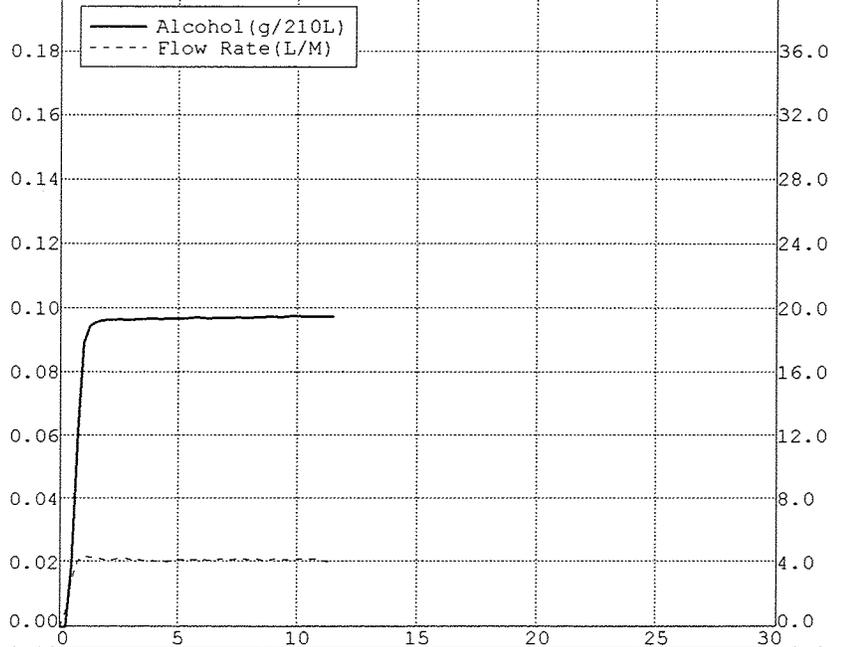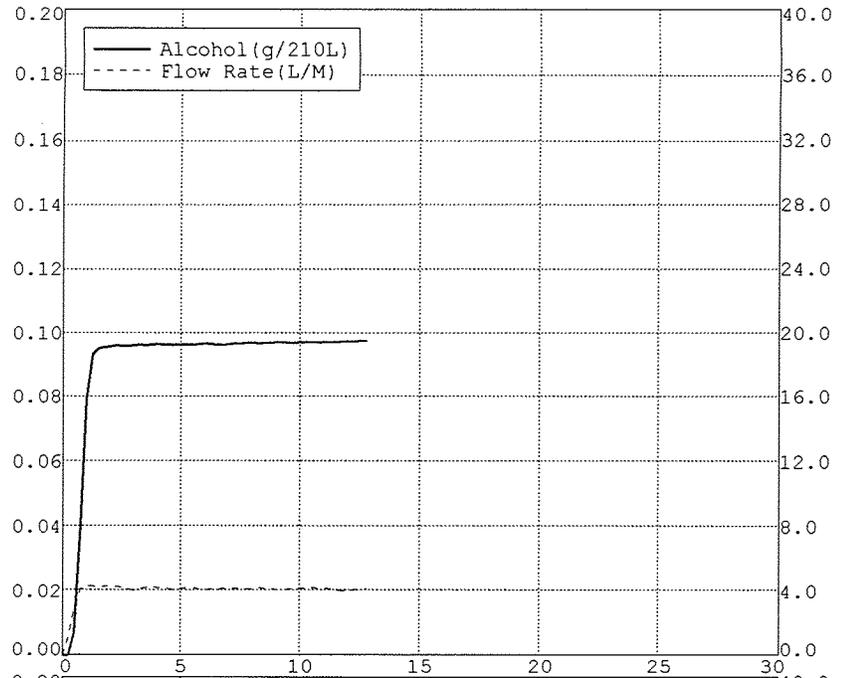

505 RLB / Bartlett case #162  
01-18-16