

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/26/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:59
INTERNAL STANDARD	VERIFIED	02:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:59
BLANK TEST	0.00	03:00
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:01
BLANK TEST	0.00	03:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:02
BLANK TEST	0.00	03:03

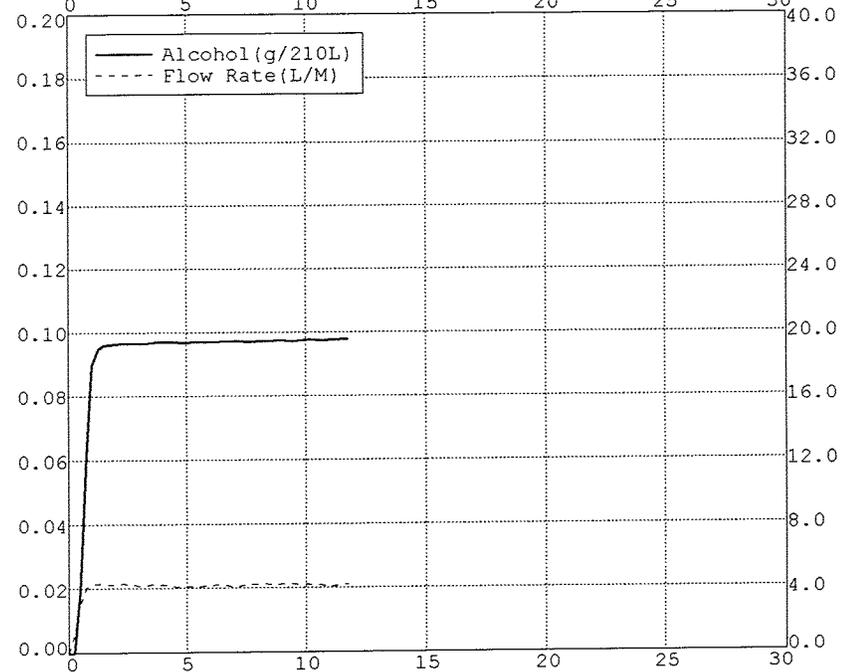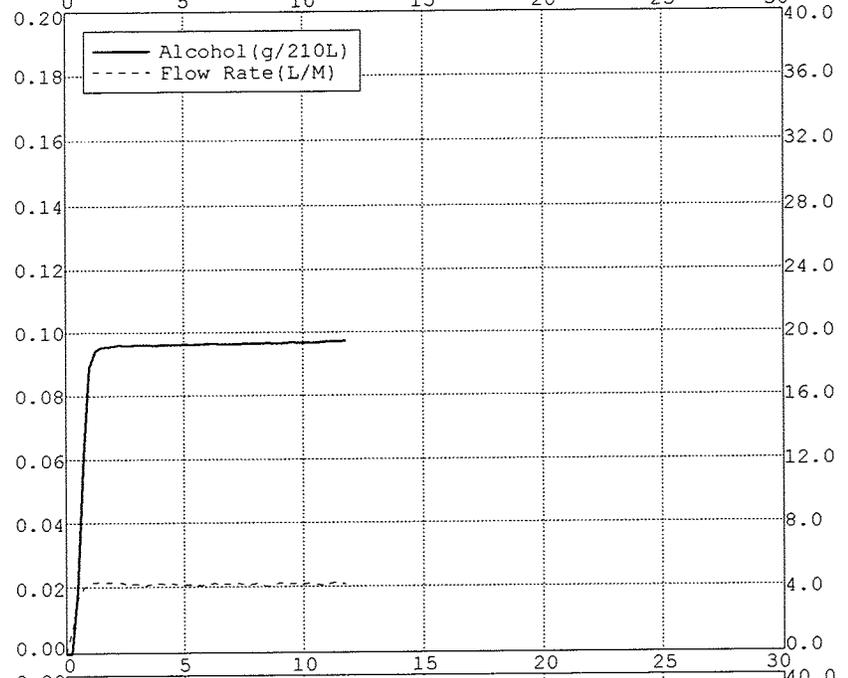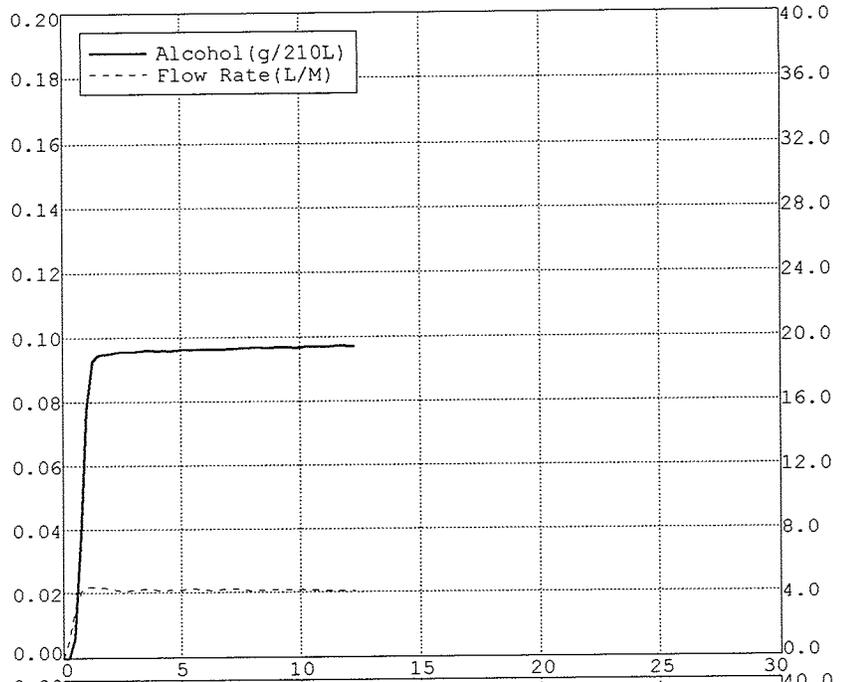

SGT *RJ Bartlett* wesc #162  
01-26-16