

SUPERVISOR TEST



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/10/2016

OPERATOR NAME:  
KENNETH W SMITH  
Permit #: 35604  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:03
INTERNAL STANDARD	VERIFIED	00:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:04
BLANK TEST	0.00	00:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:06
BLANK TEST	0.00	00:07

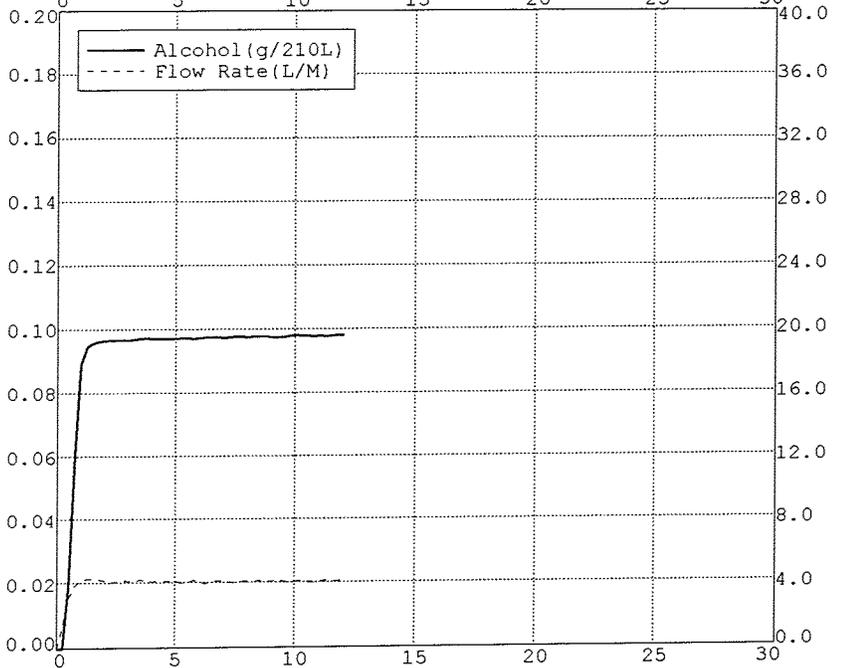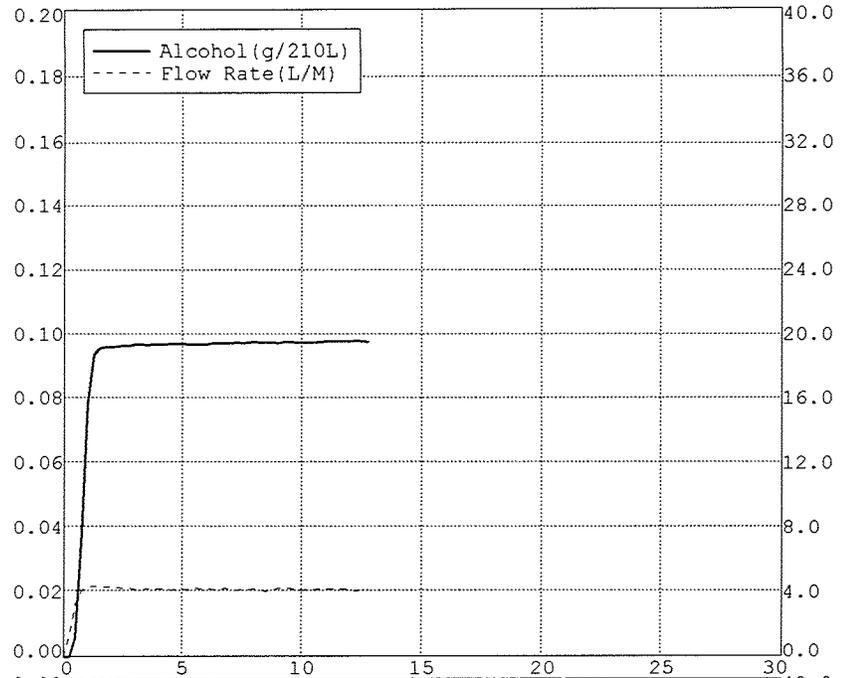

*Kenneth W. Smith*  
Kenneth W. Smith  
2/10/16

*Chester town*