

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/17/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:33
INTERNAL STANDARD	VERIFIED	10:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:34
BLANK TEST	0.00	10:35
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:35
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:37

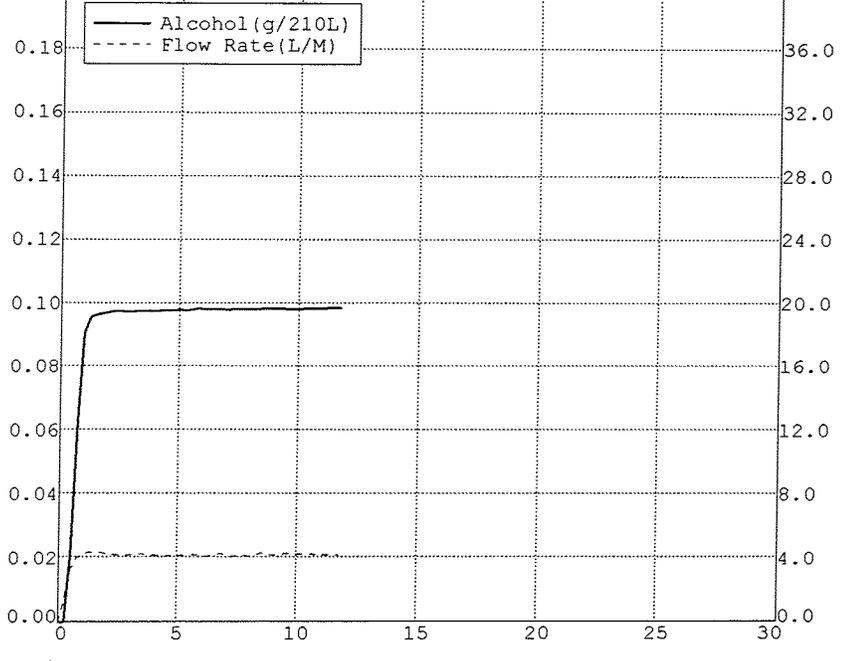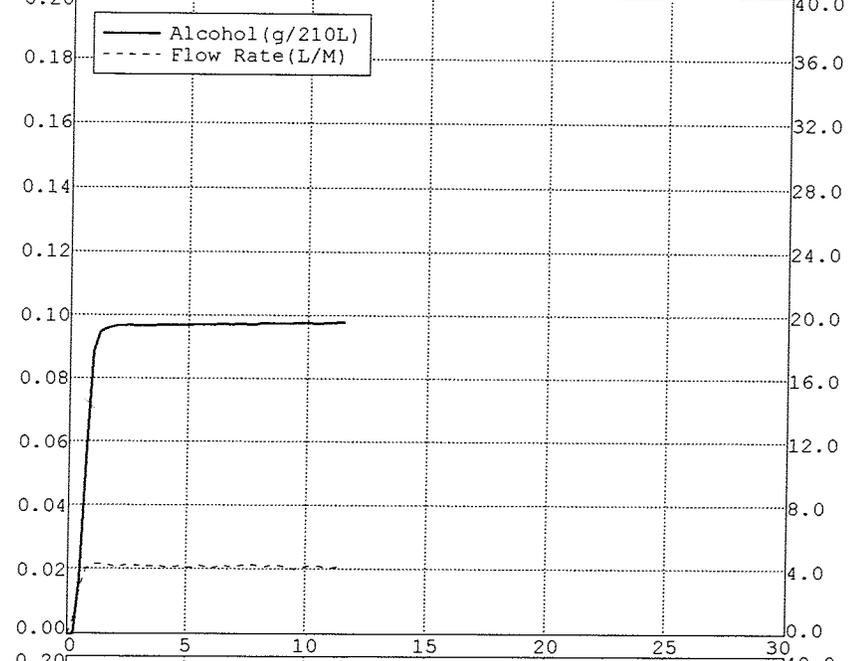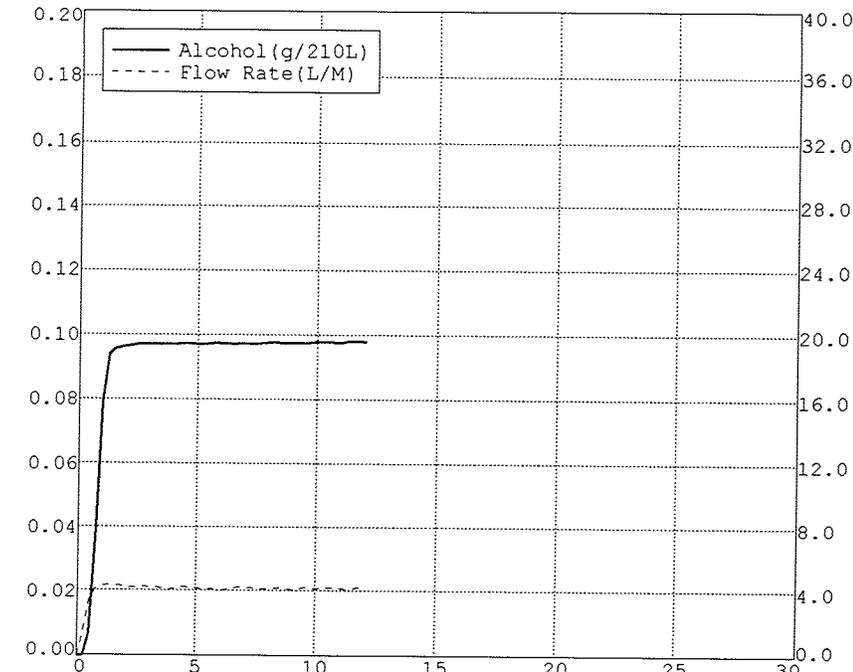

SGS RLL / Bartlett weso #162
02-17-16