

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/23/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:42
INTERNAL STANDARD	VERIFIED	02:43
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:43
BLANK TEST	0.00	02:44
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:44
BLANK TEST	0.00	02:45
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	02:46
BLANK TEST	0.00	02:46

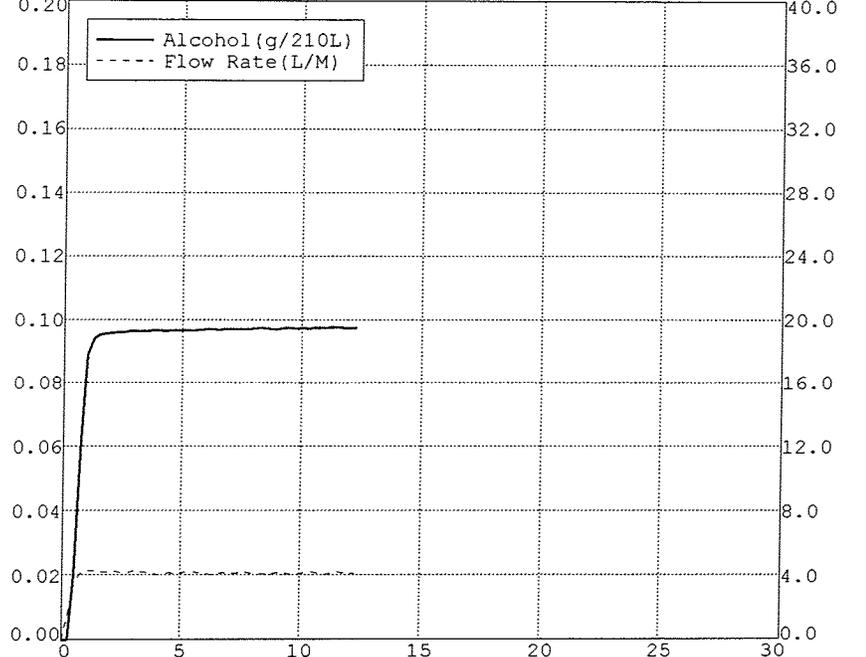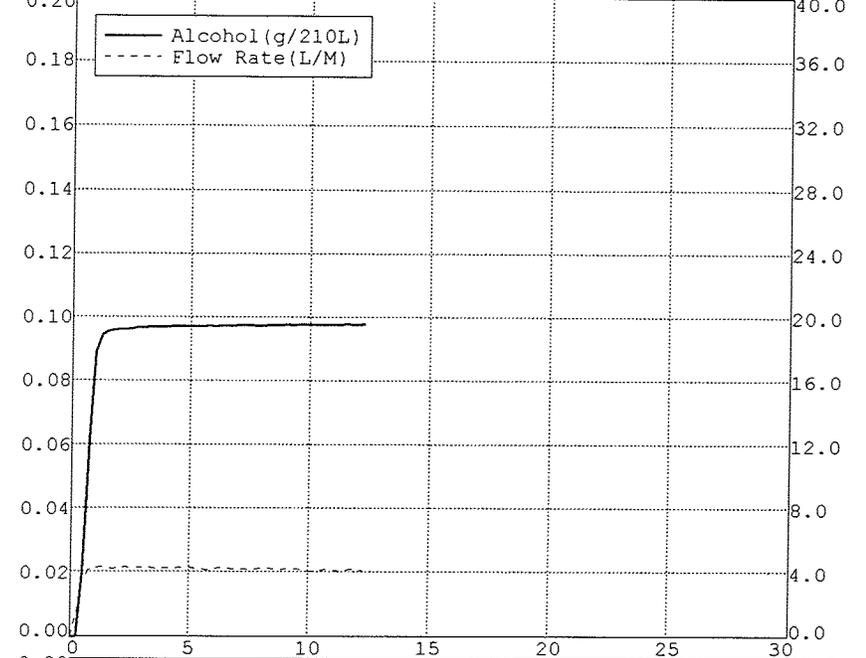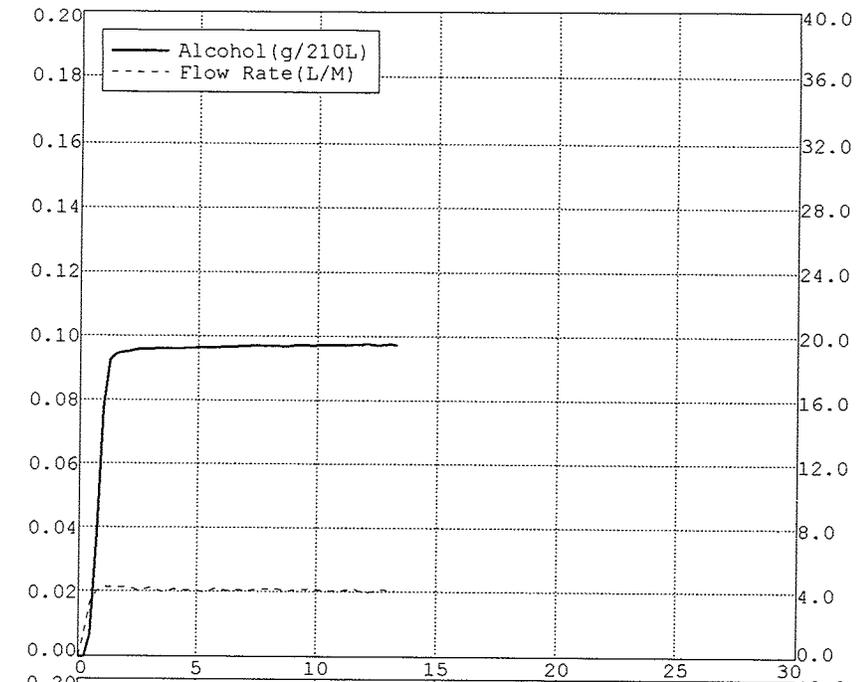

SGT Ralph Bartlett WCSO #162

02-23-16