

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 02/29/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:13
INTERNAL STANDARD	VERIFIED	03:13
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:13
BLANK TEST	0.00	03:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:15
BLANK TEST	0.00	03:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:16
BLANK TEST	0.00	03:17

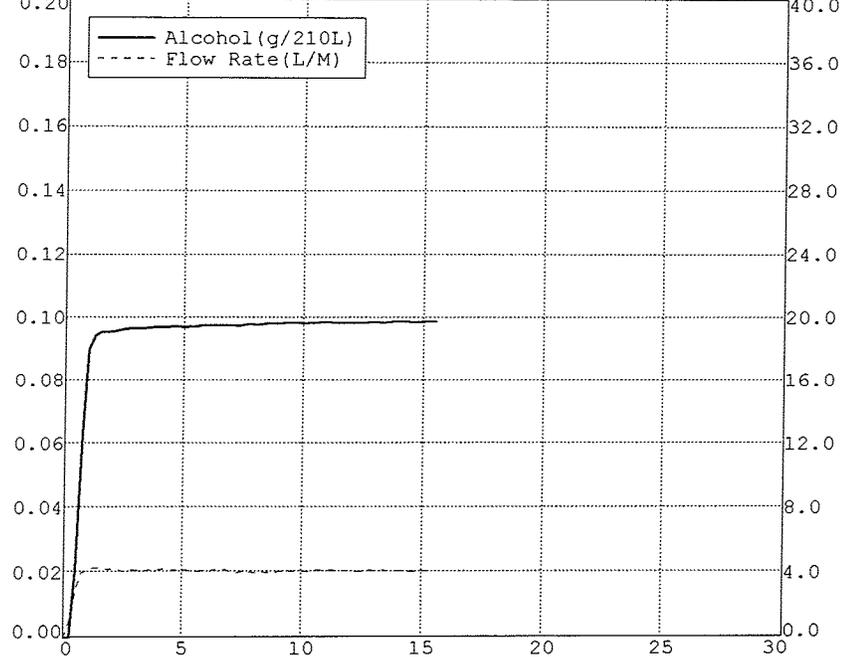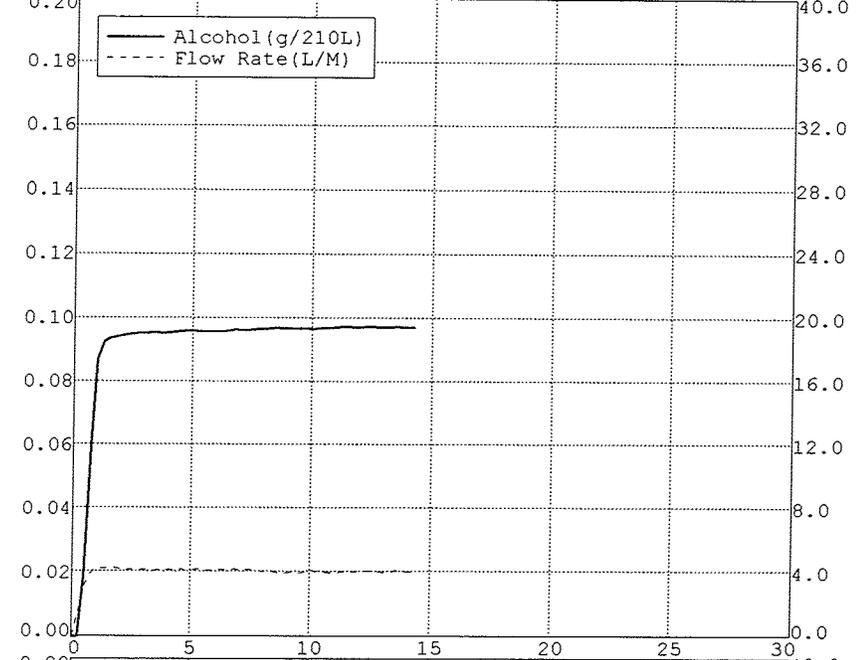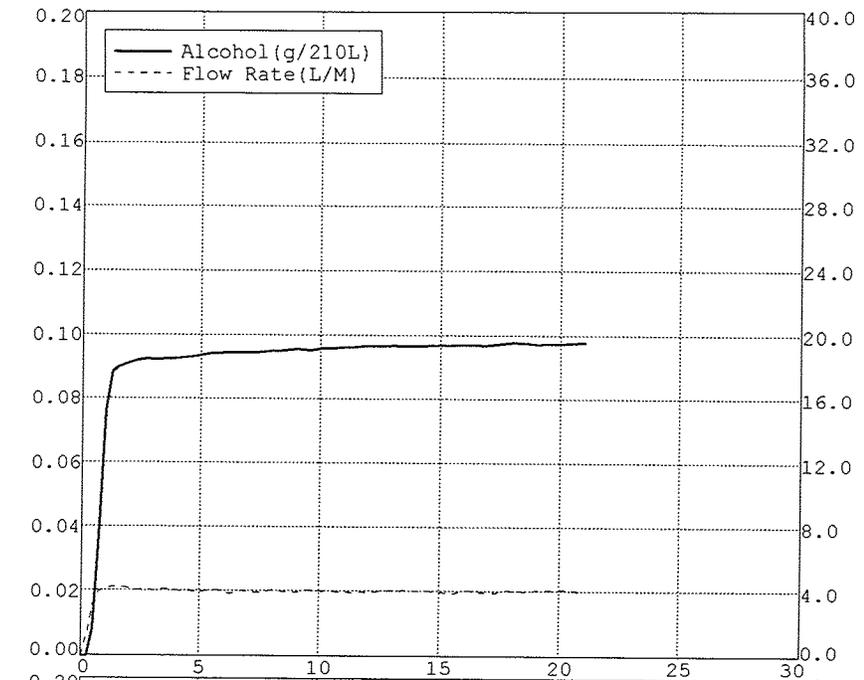

SGS *Ralph J Bartlett* WISO #162
 02-29-16