

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/08/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:05
INTERNAL STANDARD	VERIFIED	01:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:06
BLANK TEST	0.00	01:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:07
BLANK TEST	0.00	01:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:08
BLANK TEST	0.00	01:09

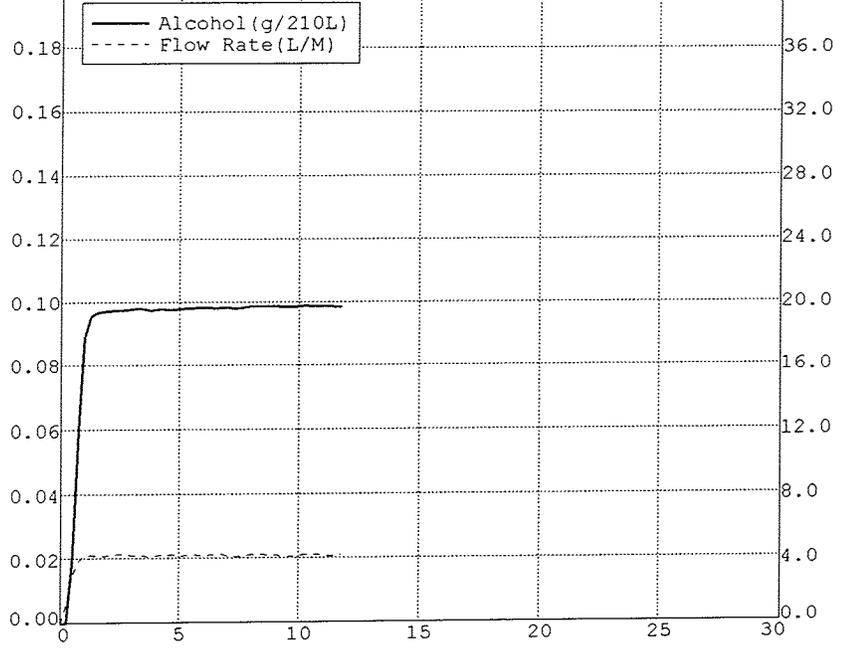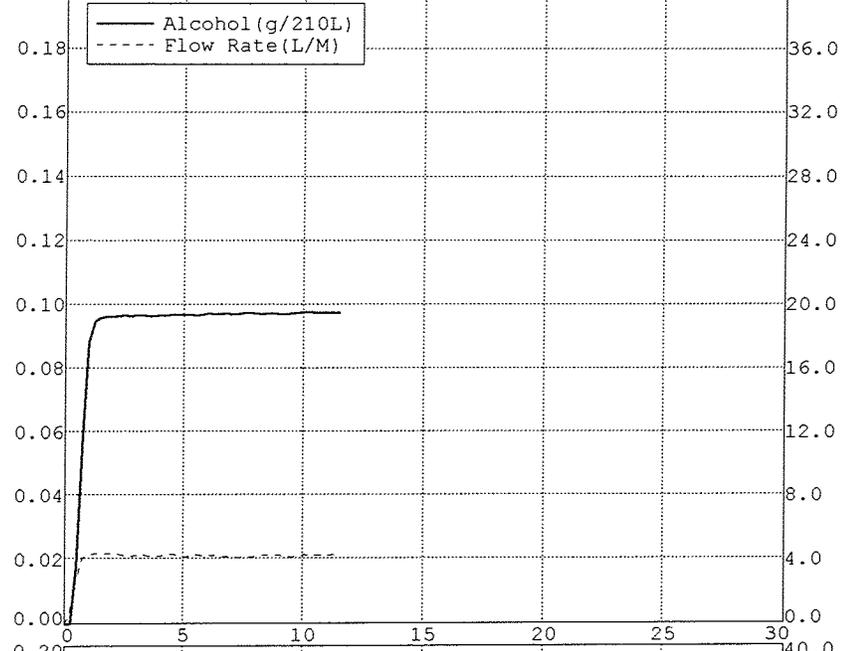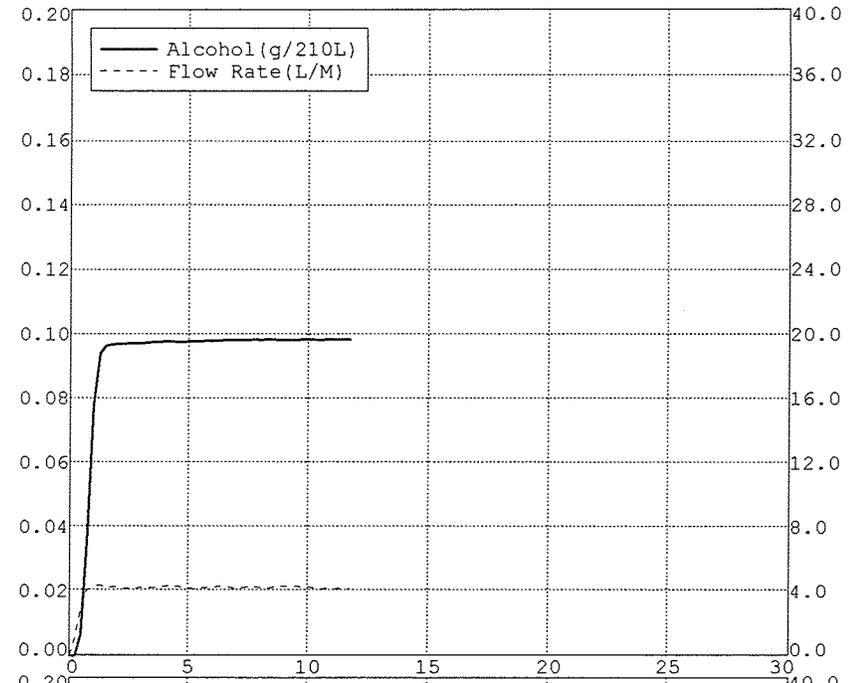

SW Red 7 Permit used #162
03-08-16