

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 03/18/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:52
INTERNAL STANDARD	VERIFIED	01:52
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:53
BLANK TEST	0.00	01:53
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:54
BLANK TEST	0.00	01:55
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	01:55
BLANK TEST	0.00	01:56

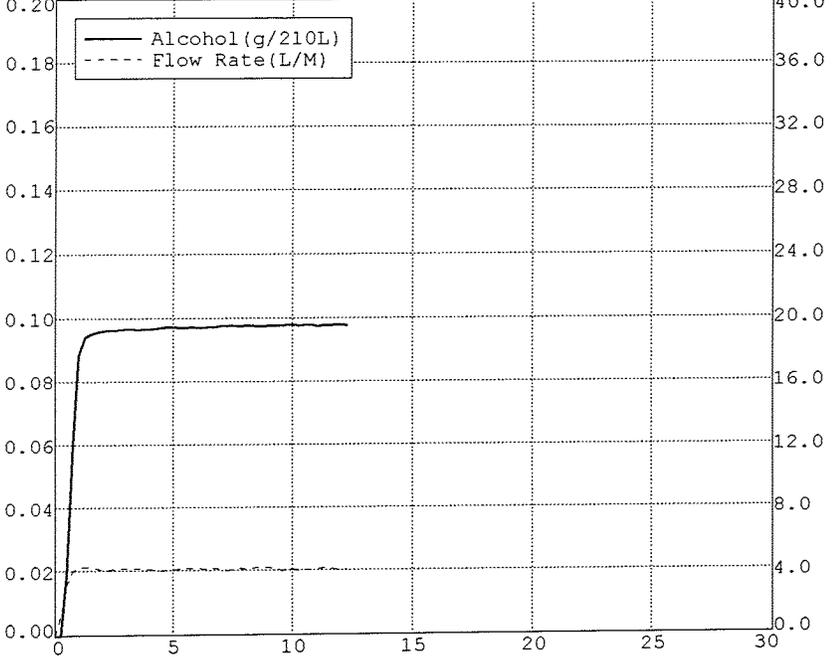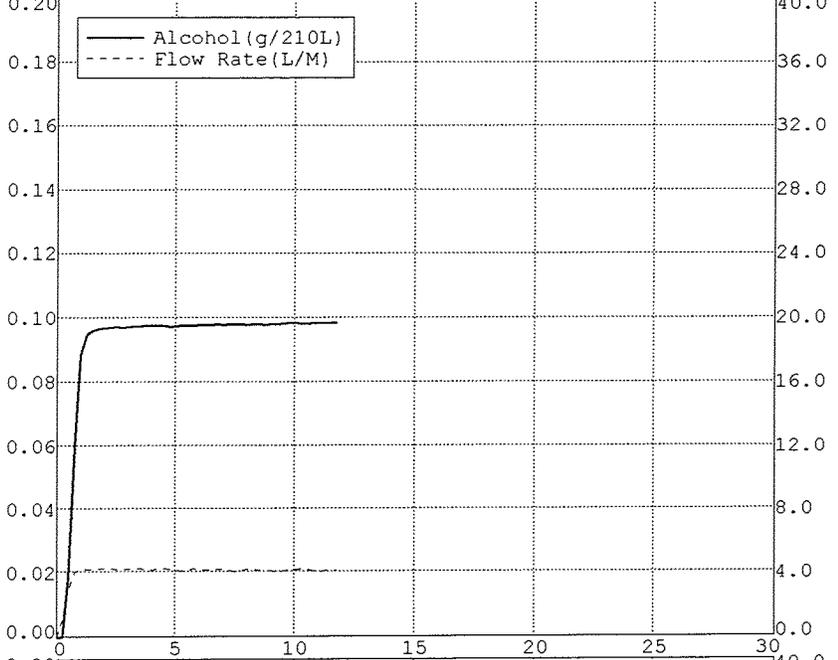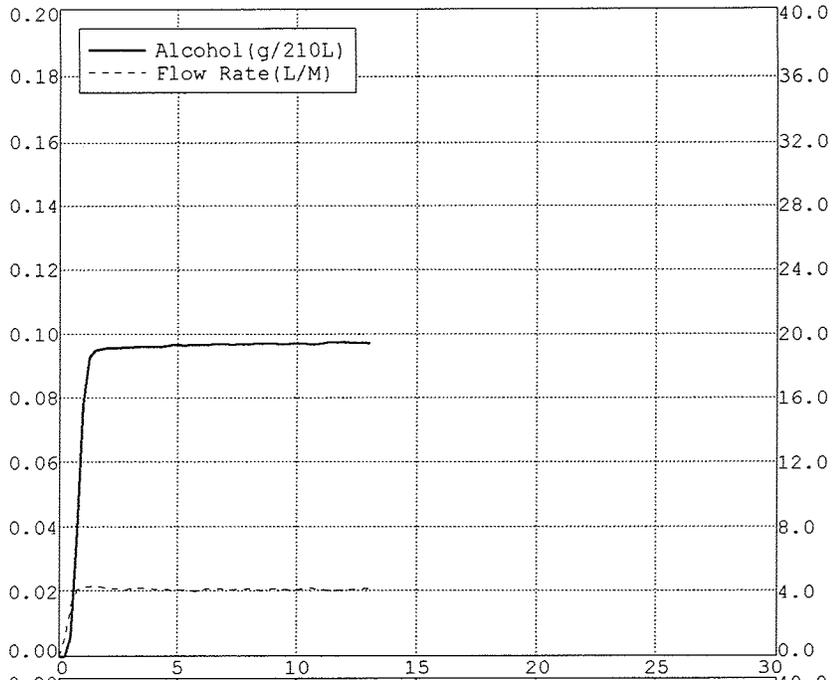

Sgt Ralph Bartlett
 WCRB #162 03-18-16