

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 03/22/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:42

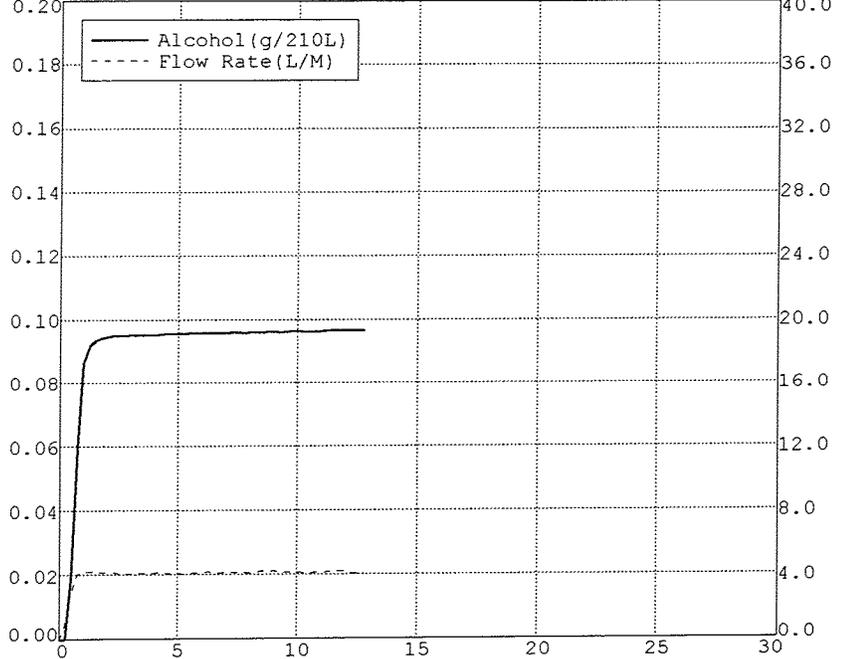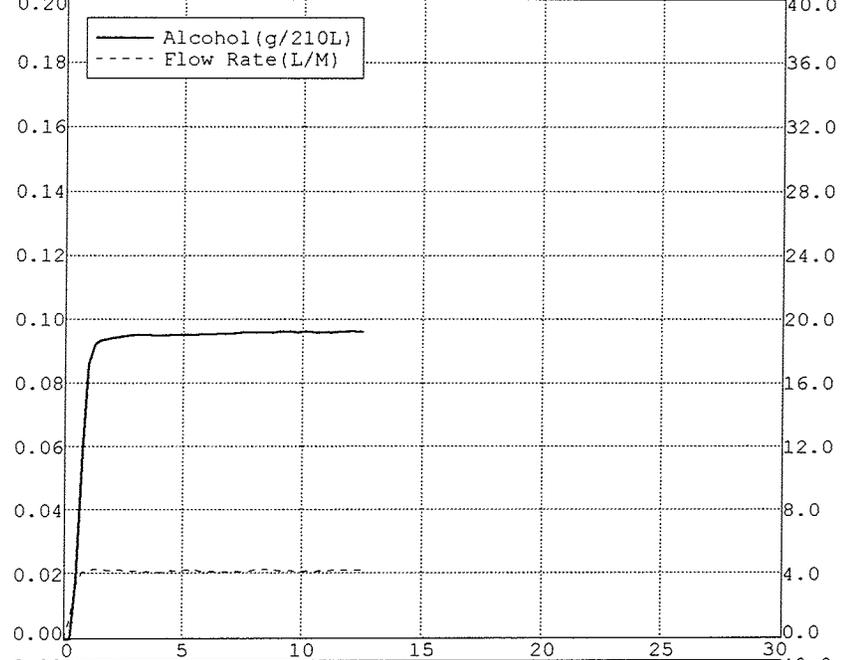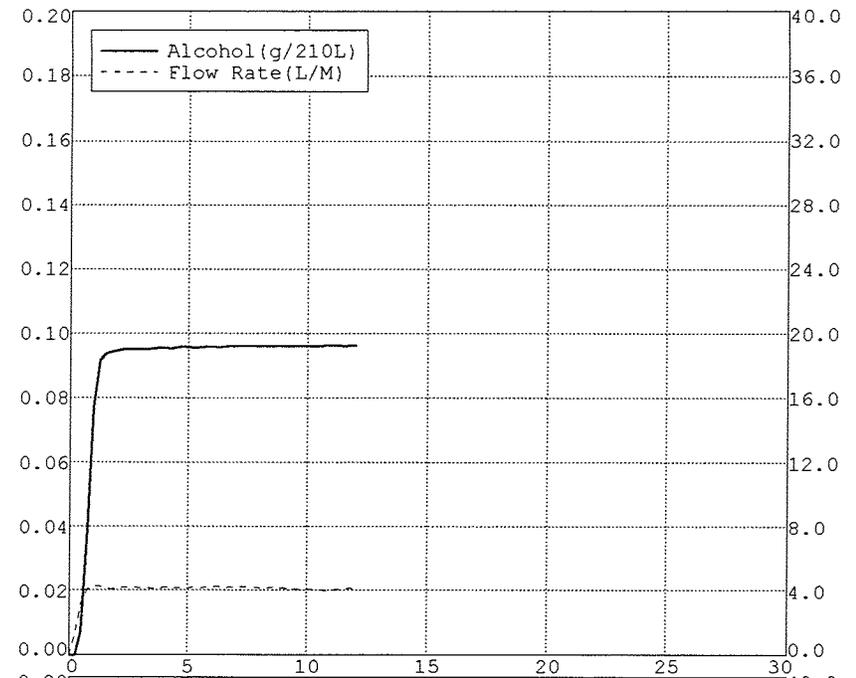

*SGS Ralph Bartlett weight #162  
03-22-16*