

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/28/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:37
INTERNAL STANDARD	VERIFIED	00:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:37
BLANK TEST	0.00	00:38
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41

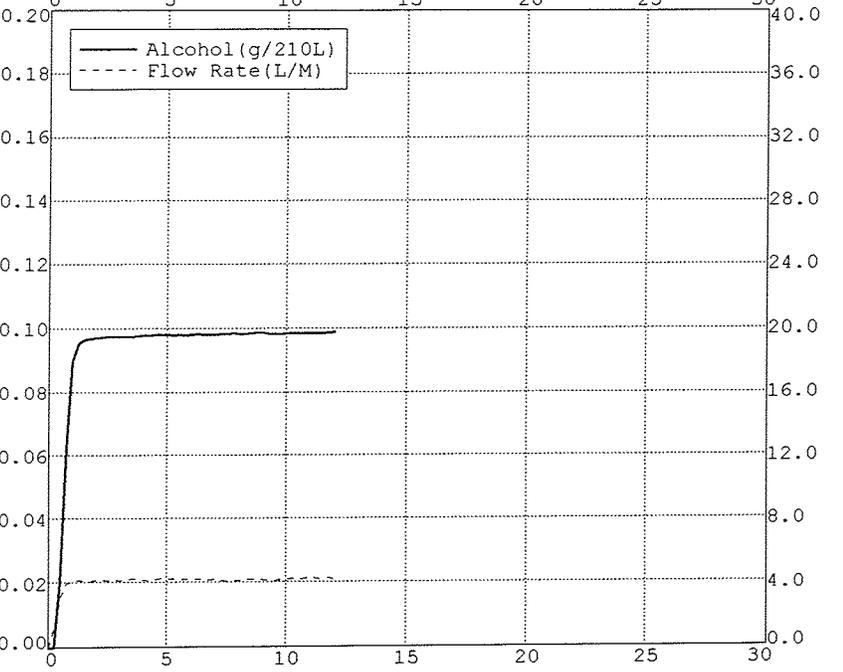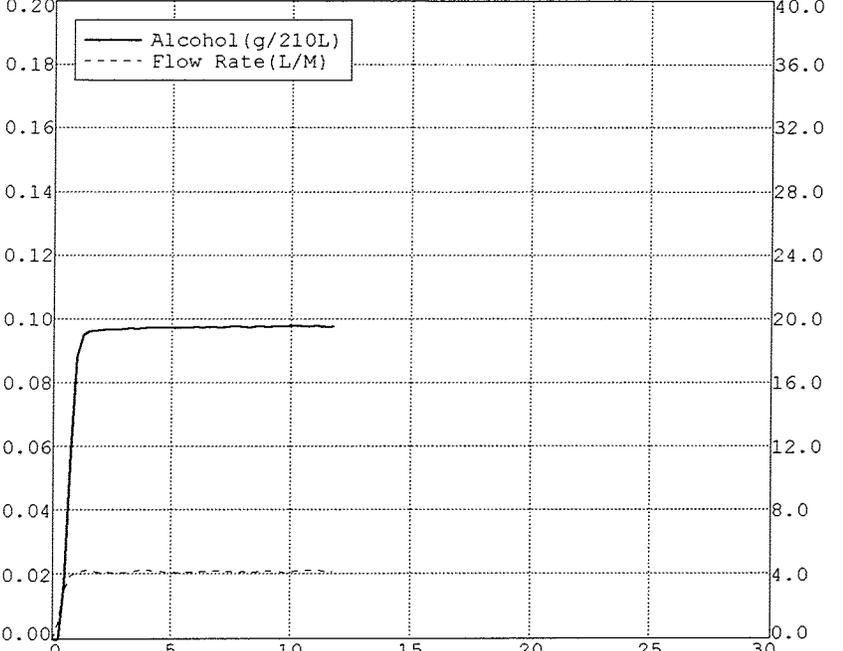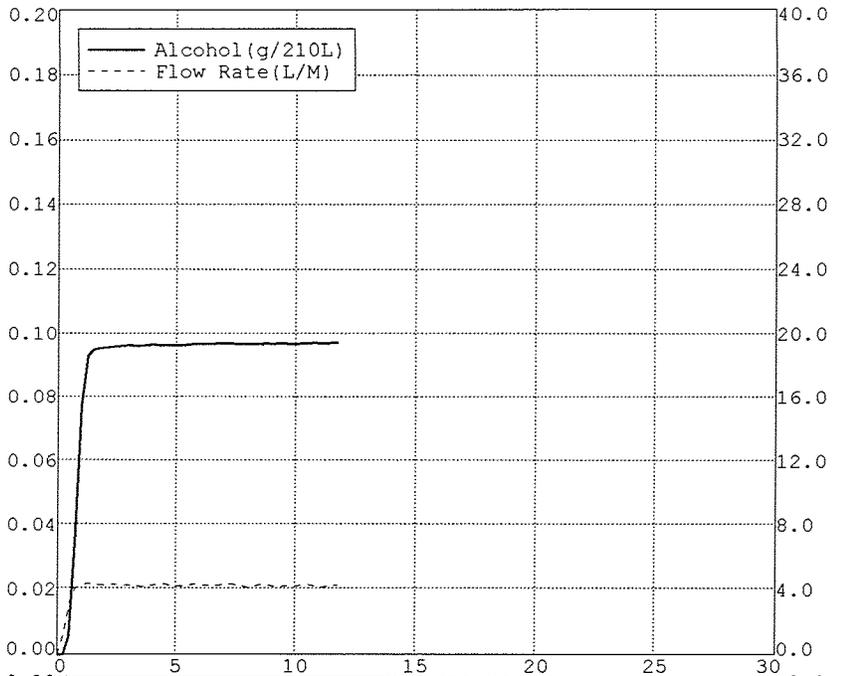

SUS Ralph J Bartlett
WCSO #162 03-28-16