

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 04/05/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:00
INTERNAL STANDARD	VERIFIED	01:00
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:01
BLANK TEST	0.00	01:02
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:02
BLANK TEST	0.00	01:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:03
BLANK TEST	0.00	01:04

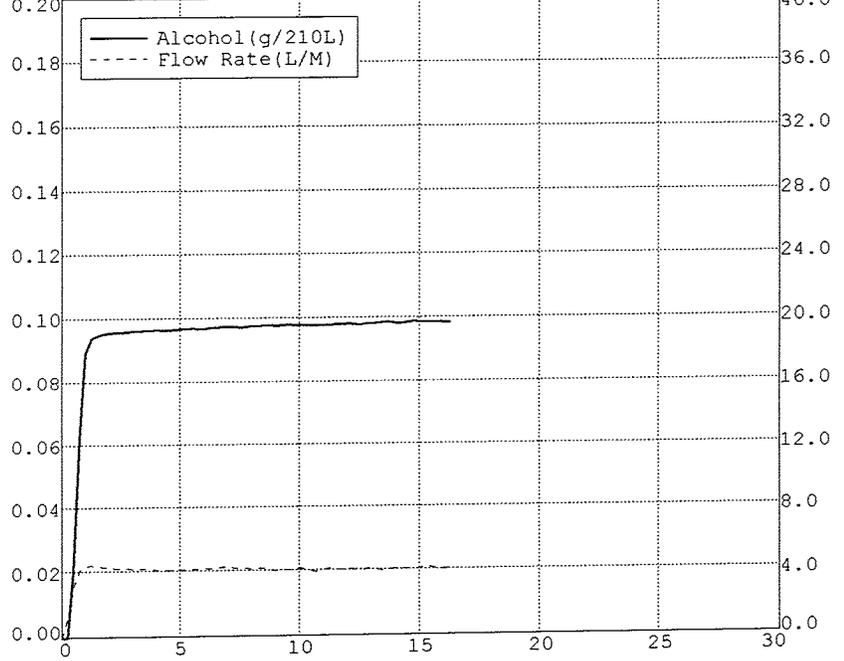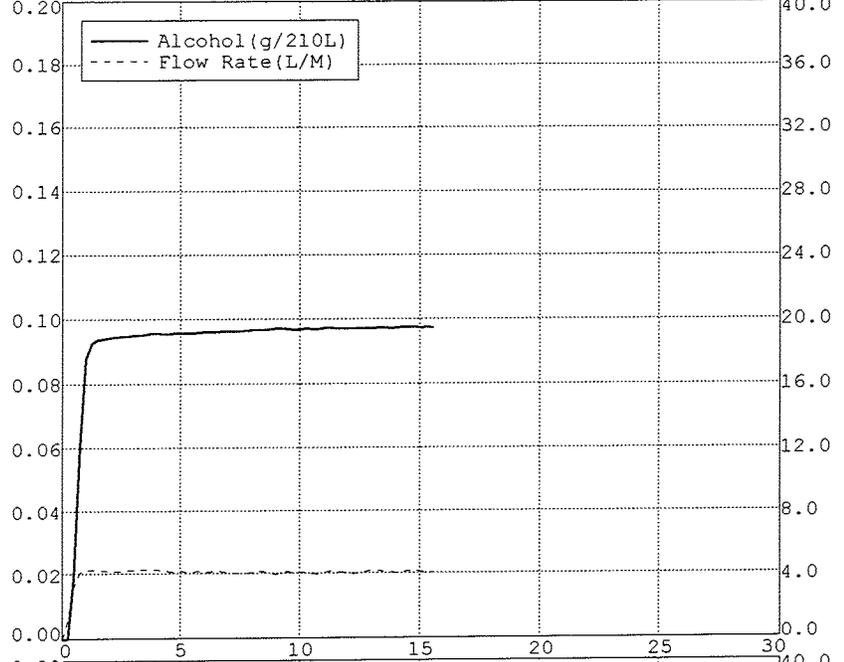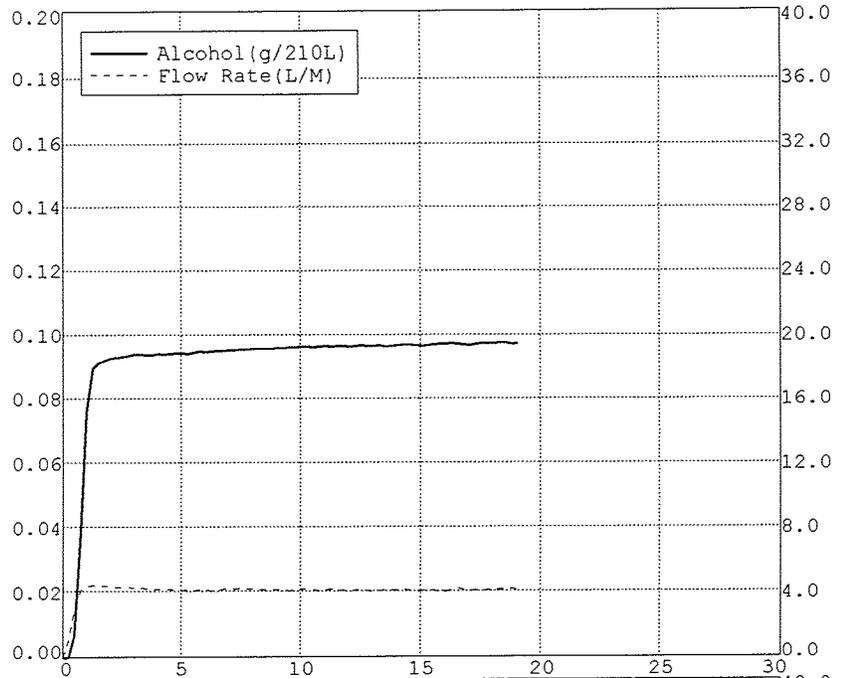

*55 Raff 1 Rates were #162  
04-05-16*