

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 04/11/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:03
INTERNAL STANDARD	VERIFIED	01:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:04
BLANK TEST	0.00	01:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:05
BLANK TEST	0.00	01:06
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	01:06
BLANK TEST	0.00	01:07

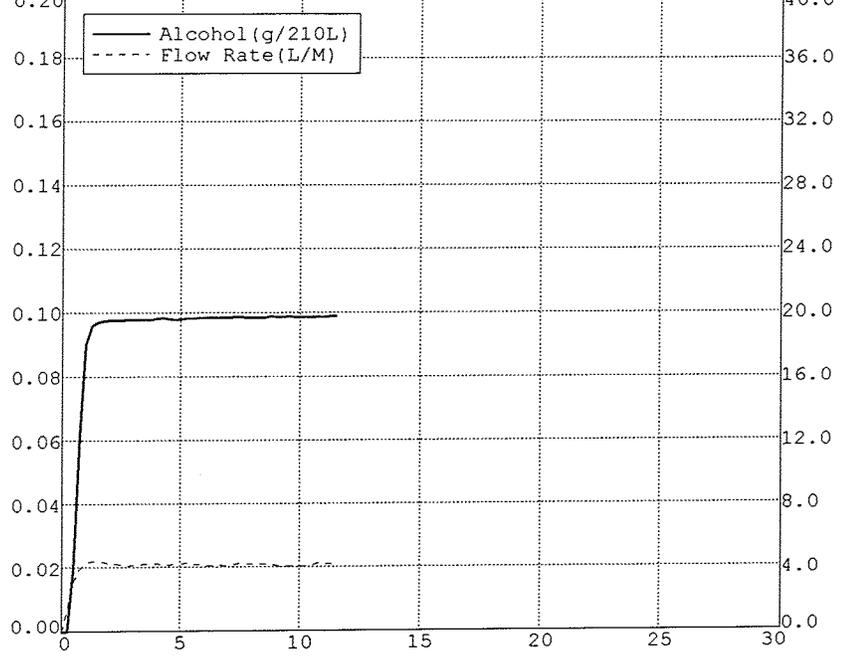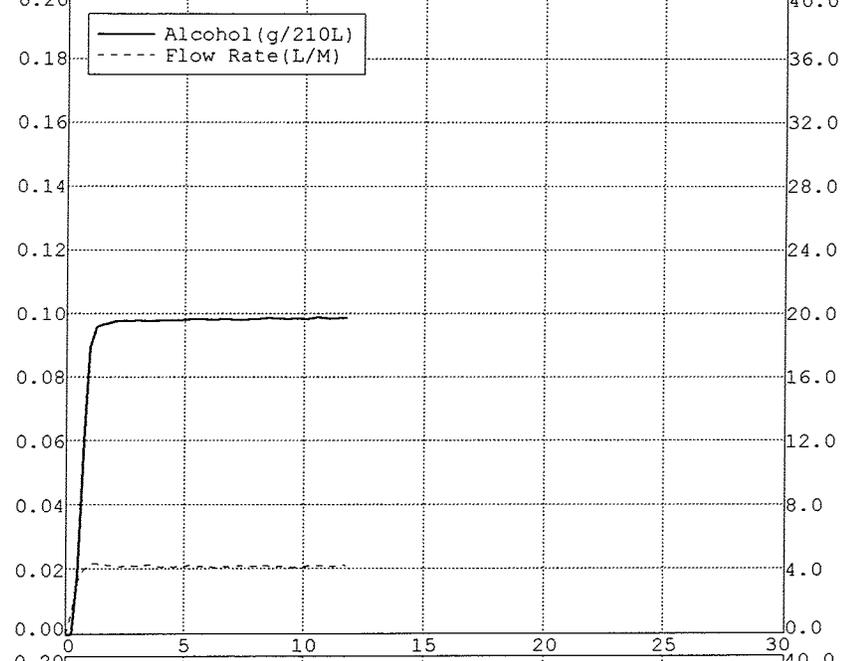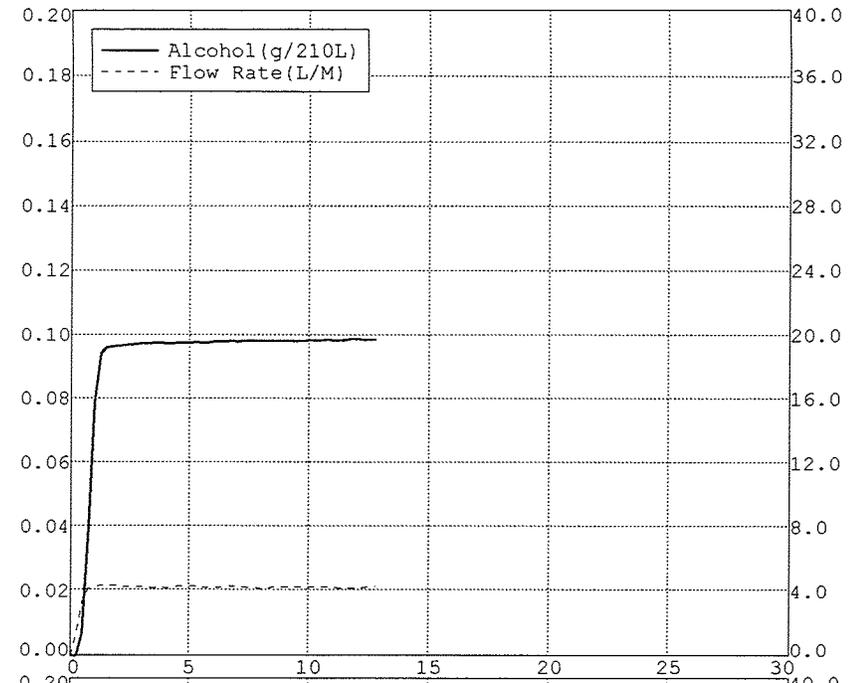

565 Ralph Bartlett Warren #162  
04-11-16