

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/19/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:57
INTERNAL STANDARD	VERIFIED	00:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:57
BLANK TEST	0.00	00:58
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:58
BLANK TEST	0.00	00:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:00
BLANK TEST	0.00	01:01

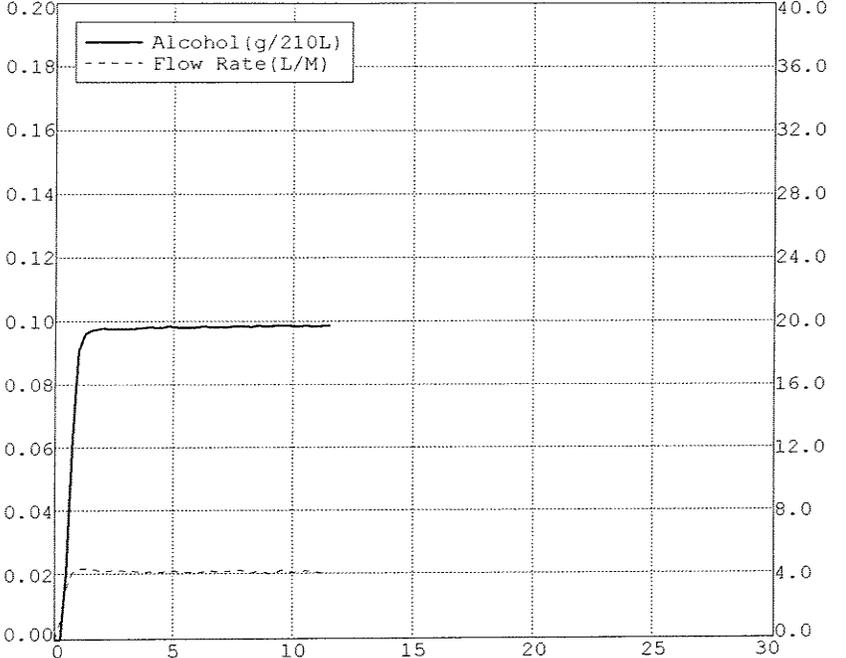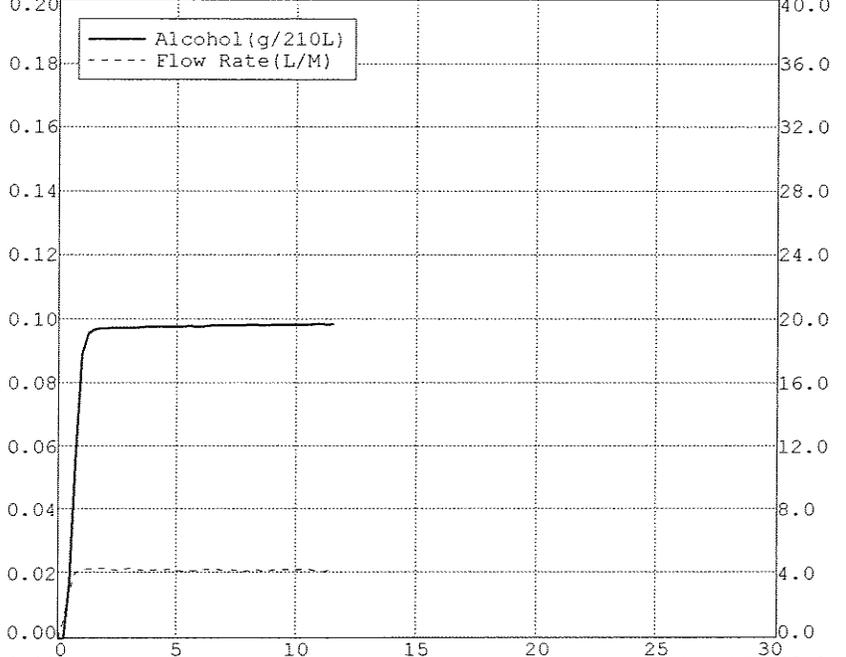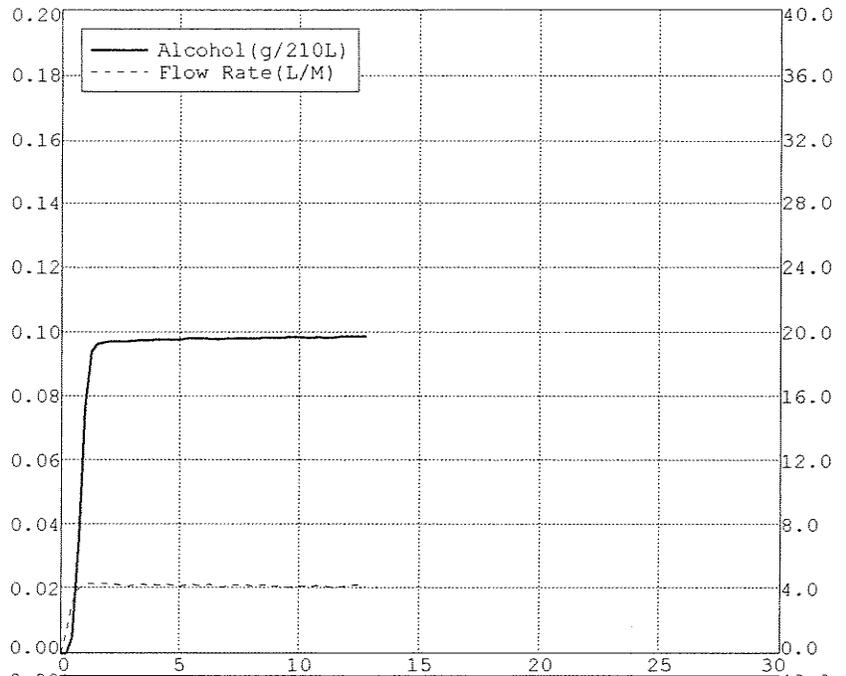

SOB R.J. Bartlett WRS # 162
04-19-16