

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 05/09/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:44
INTERNAL STANDARD	VERIFIED	00:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:45
BLANK TEST	0.00	00:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:46
BLANK TEST	0.00	00:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:48

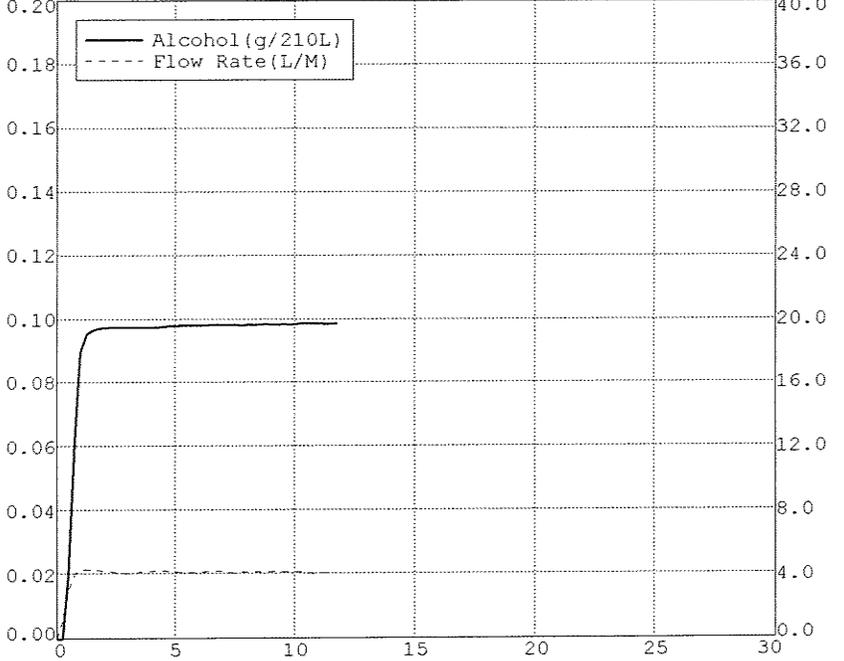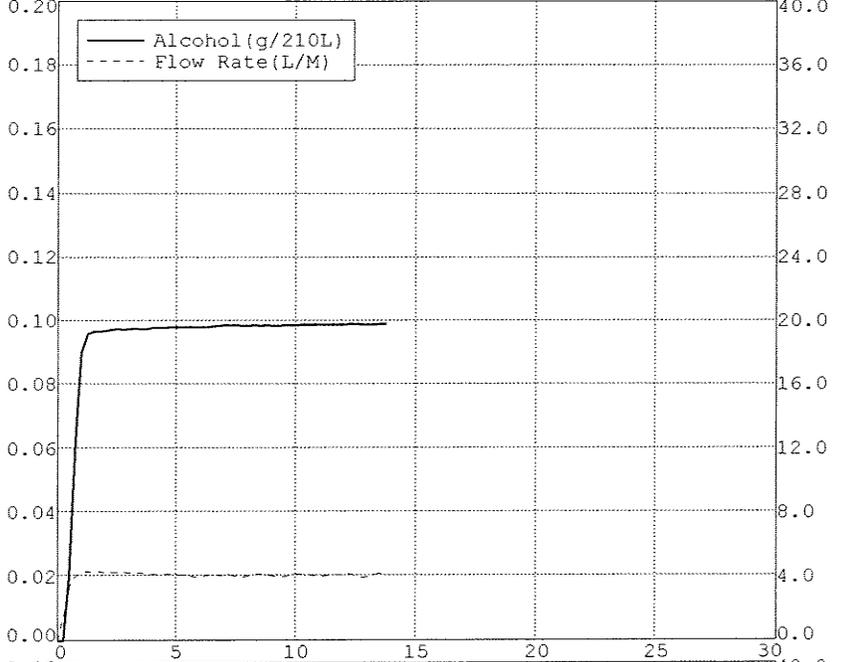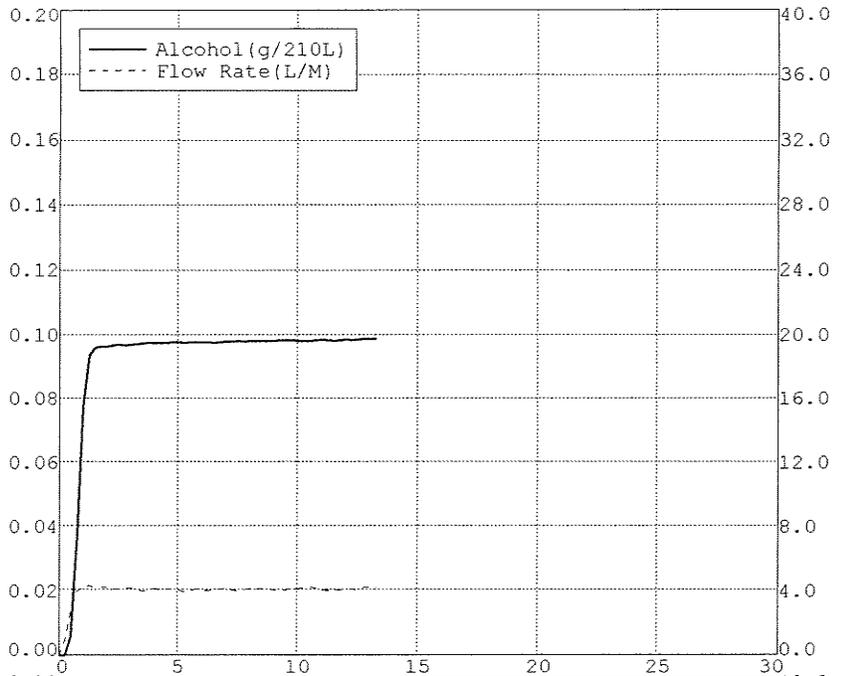

SOS Dept of Justice case # 102  
05-09-16