

SUPERVISOR TEST



WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/22/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16050

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 23:13 |
| INTERNAL STANDARD | VERIFIED | 23:13 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 23:13 |
| BLANK TEST | 0.00 | 23:14 |
| REFERENCE STANDARD TEMP | 33.96c | |
| REFERENCE STANDARD | 0.09 | 23:14 |
| BLANK TEST | 0.00 | 23:15 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 23:16 |
| BLANK TEST | 0.00 | 23:17 |

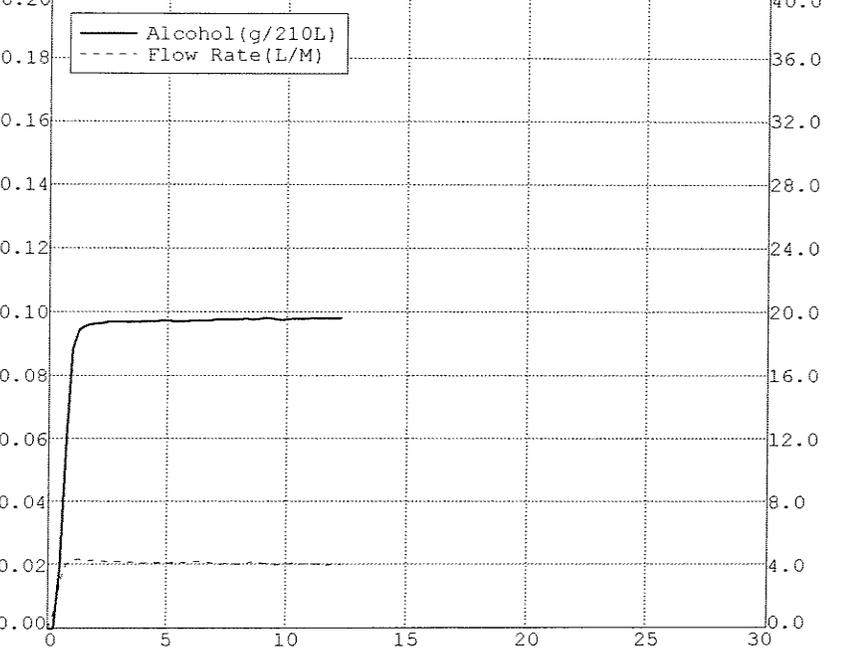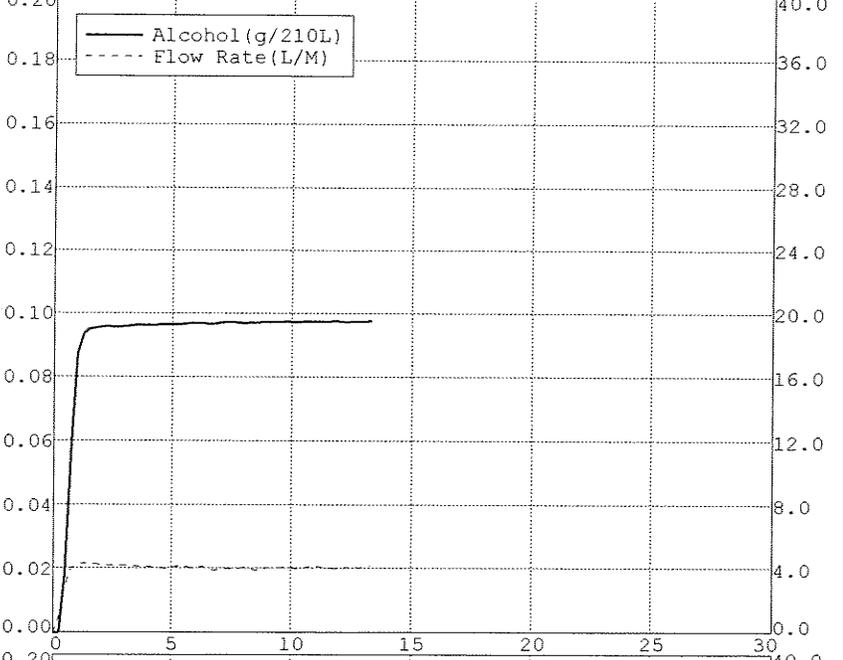

SGS Ralph J Bartlett 105208/16
 05-22-16