

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/01/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:46
INTERNAL STANDARD	VERIFIED	00:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:48
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:51

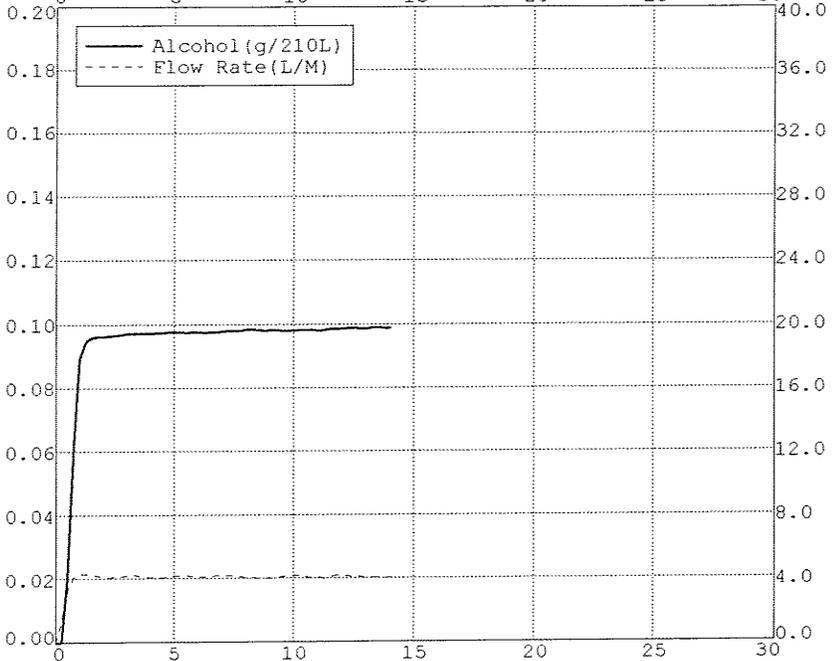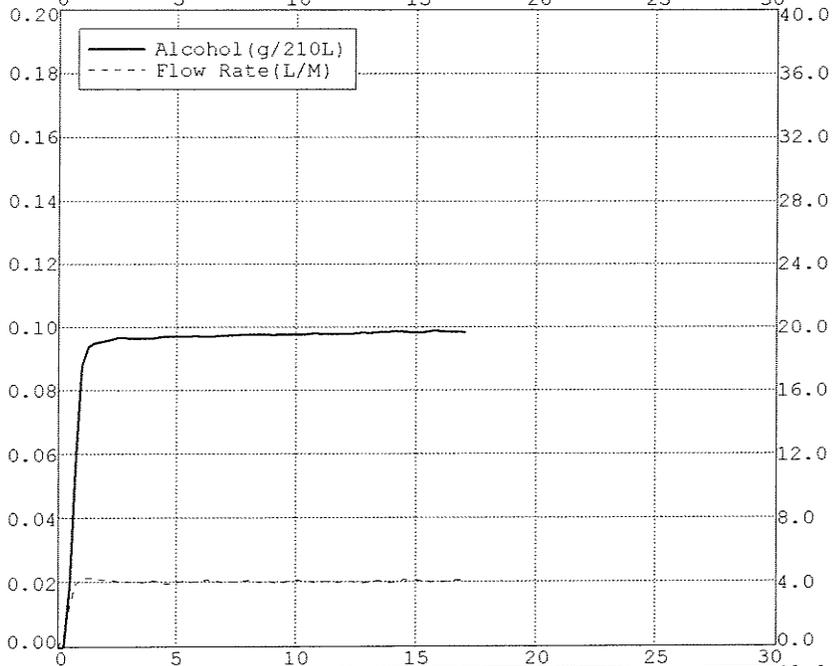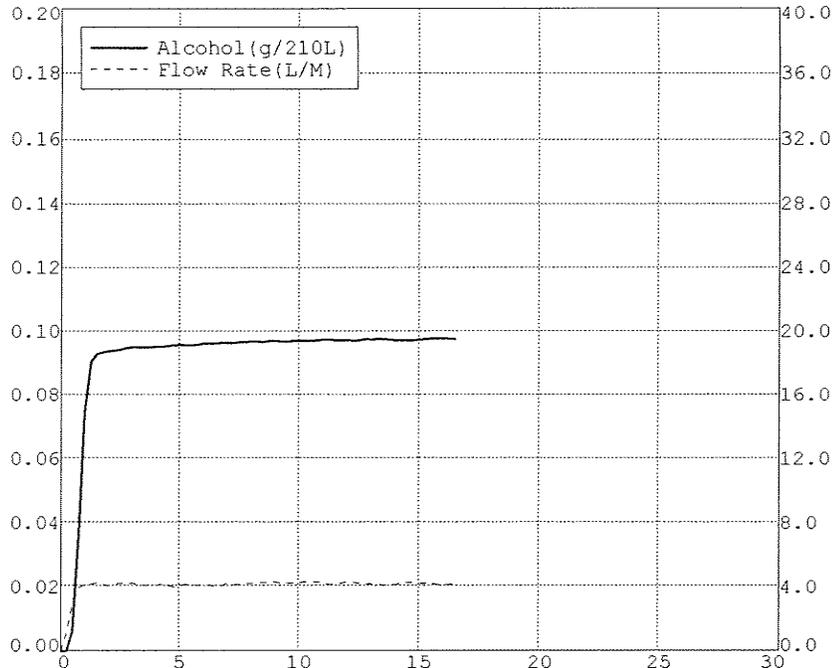

507 Ref. Run # 16090
06/01/16