

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/06/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:07
INTERNAL STANDARD	VERIFIED	02:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:08
BLANK TEST	0.00	02:09
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	02:09
BLANK TEST	0.00	02:10
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	02:11
BLANK TEST	0.00	02:12

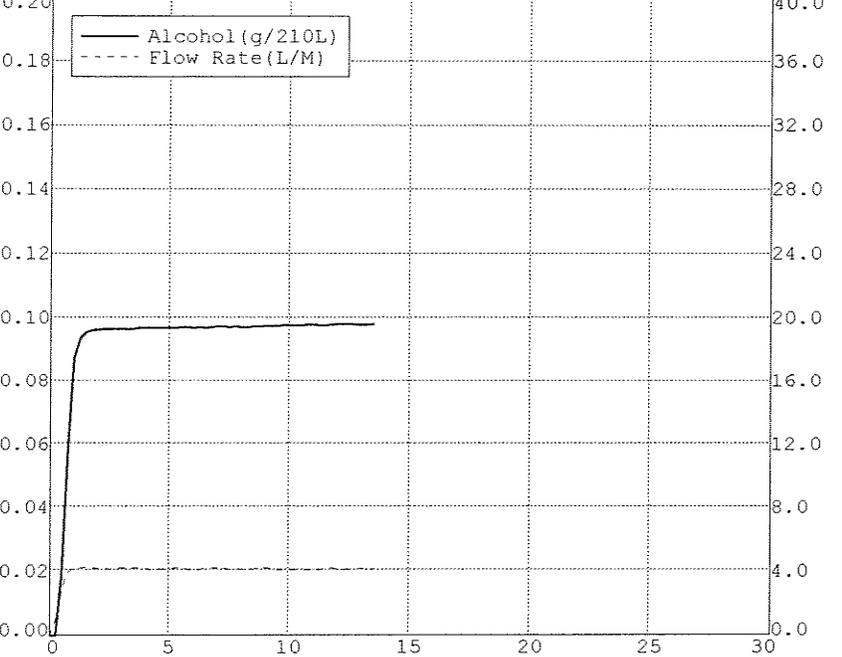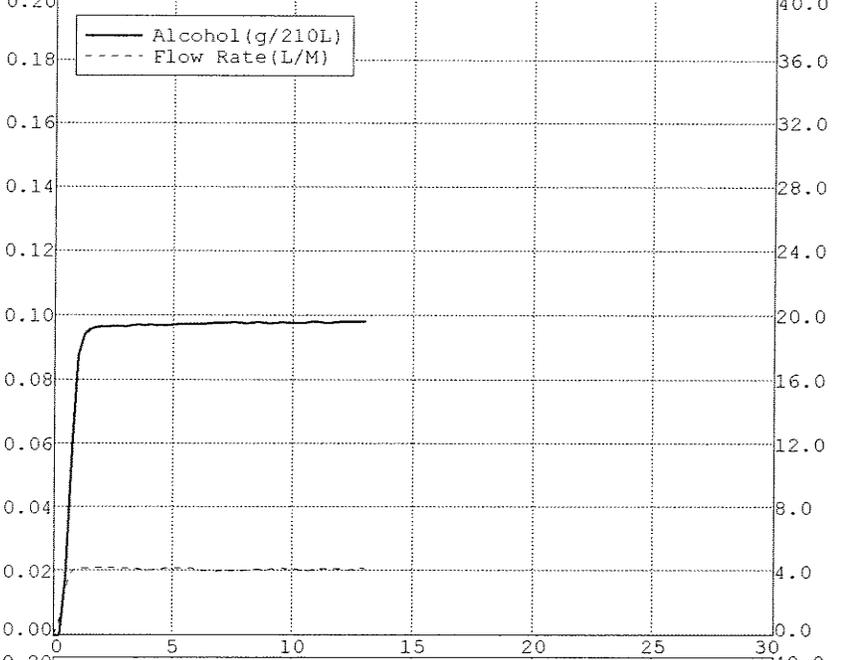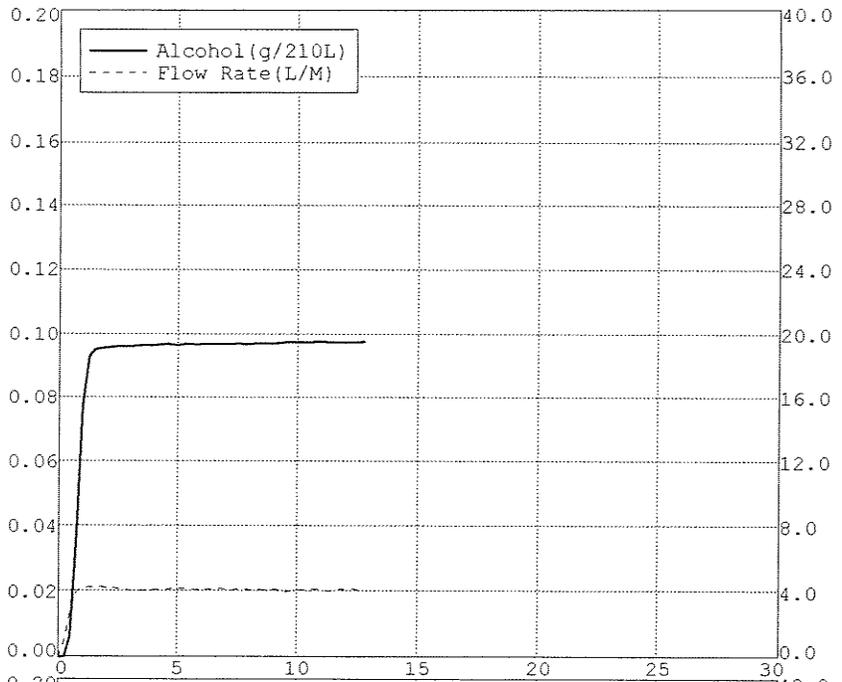

See Ralph J Bartlett
06-06-16
wco #162