

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 06/28/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:01
INTERNAL STANDARD	VERIFIED	01:01
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:01
BLANK TEST	0.00	01:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:02
BLANK TEST	0.00	01:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:04
BLANK TEST	0.00	01:05

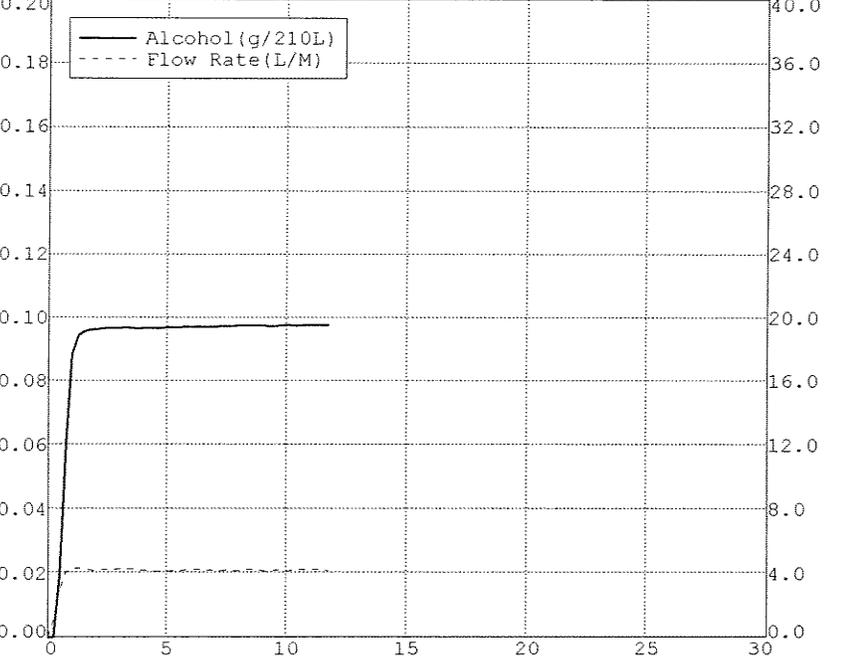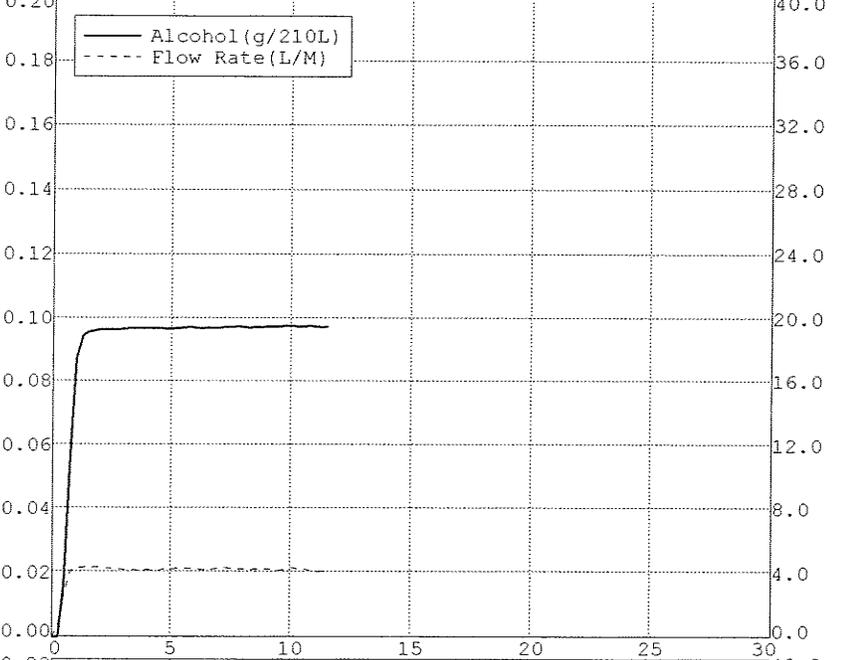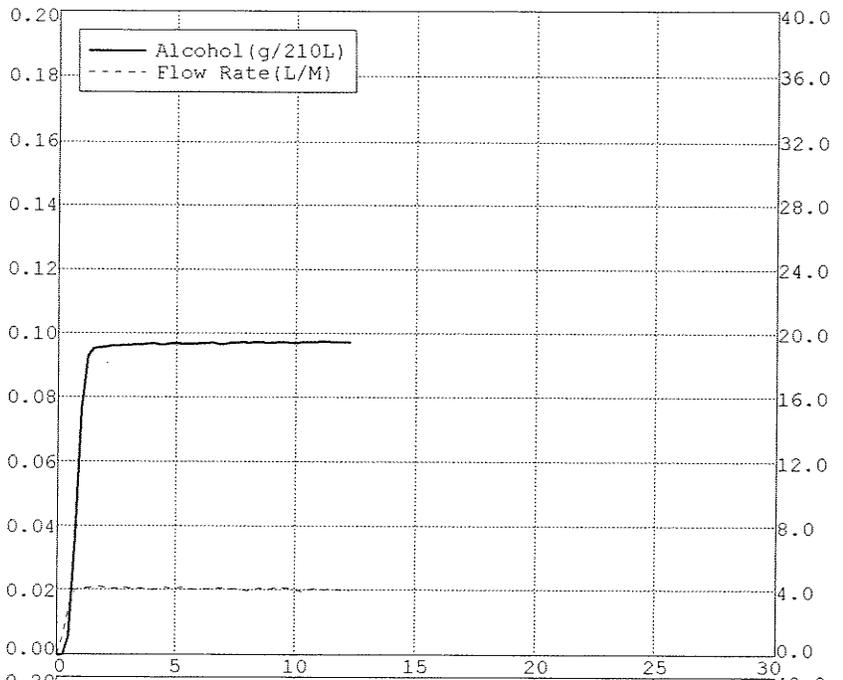

SGR Ralph J Bartlett W050#16
 06-28-16