

SOLUTION CHANGE



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/04/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:17
INTERNAL STANDARD	VERIFIED	01:17
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:17
BLANK TEST	0.00	01:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:19
BLANK TEST	0.00	01:20
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:20
BLANK TEST	0.00	01:21

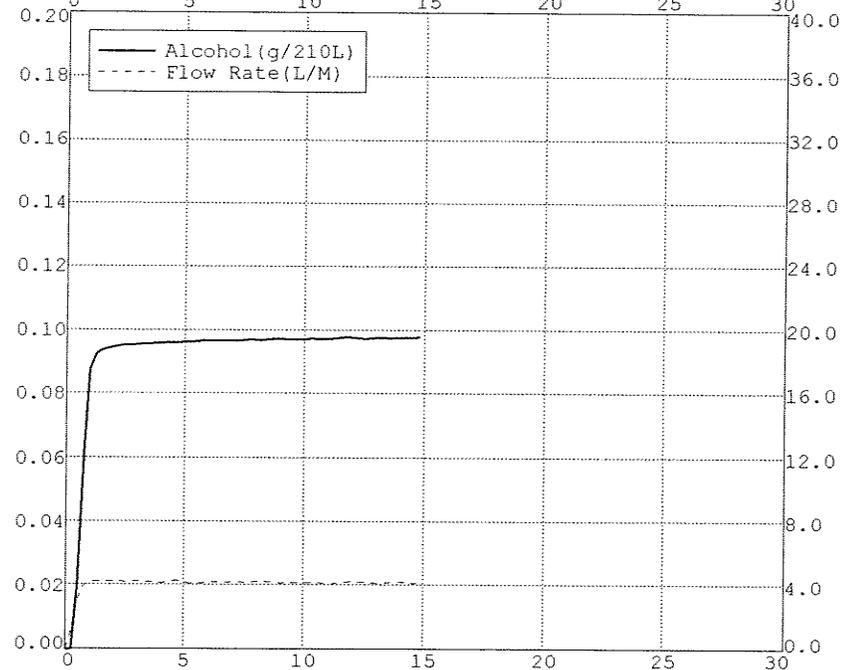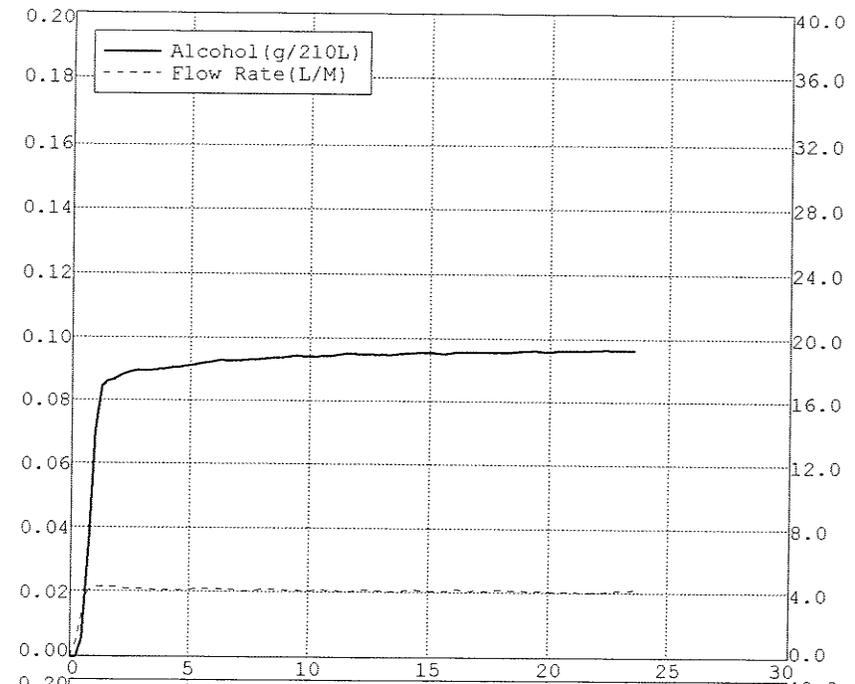

SCS *RJ Bartlett* WSO #162
07-04-16