

SOLUTION CHANGE




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 08/01/2016

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:11
INTERNAL STANDARD	VERIFIED	02:11
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:12
BLANK TEST	0.00	02:13
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	02:13
BLANK TEST	0.00	02:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:15
BLANK TEST	0.00	02:16

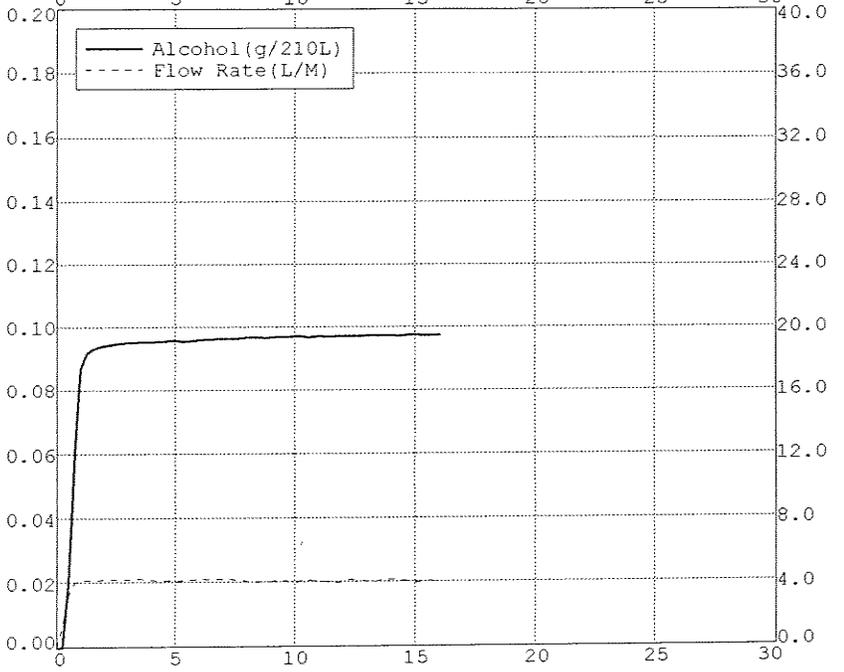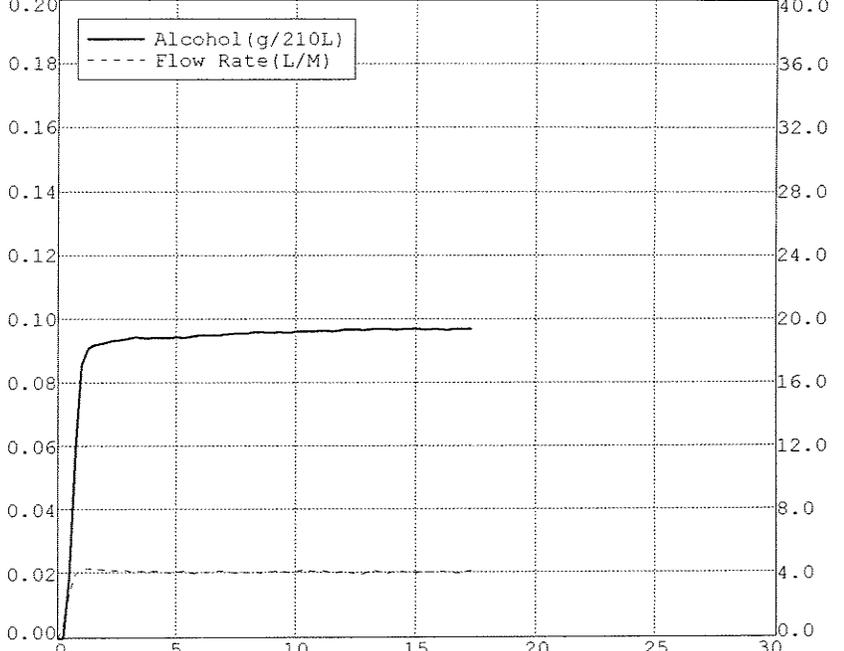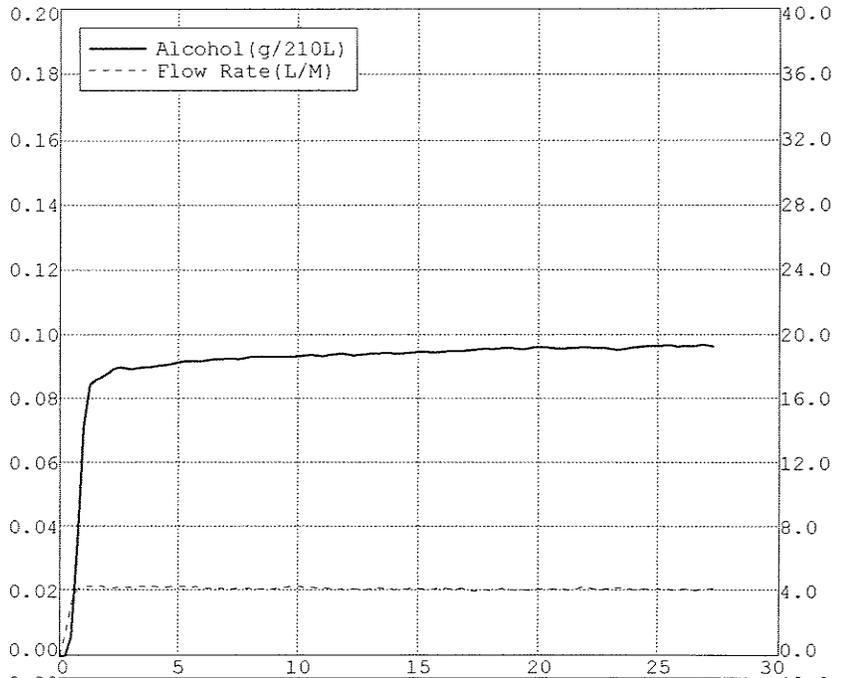

*See Ralph Bartlett*  
 Wc10 # 162 08-01-16