

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 08/09/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:52
INTERNAL STANDARD	VERIFIED	00:52
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:52
BLANK TEST	0.00	00:53
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:55
BLANK TEST	0.00	00:56

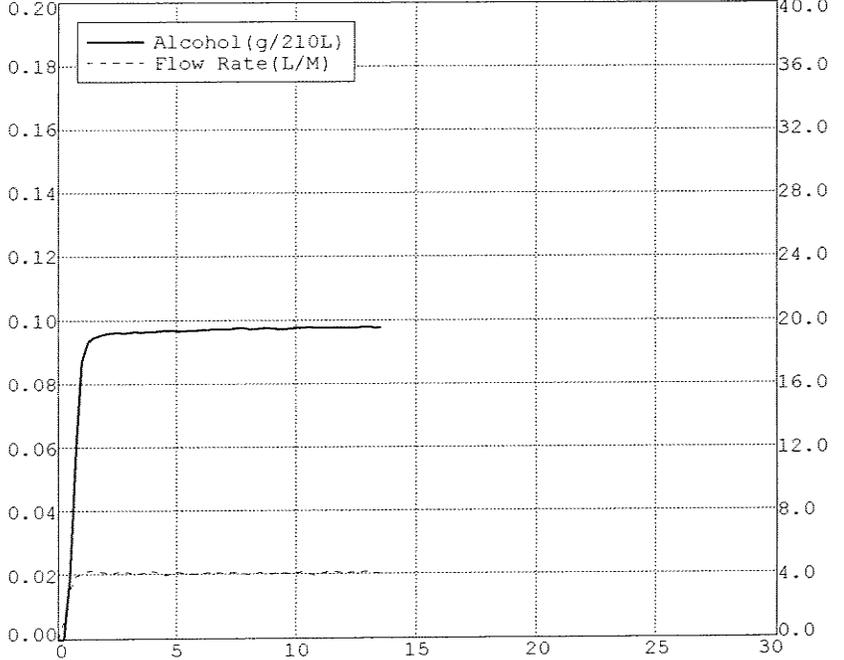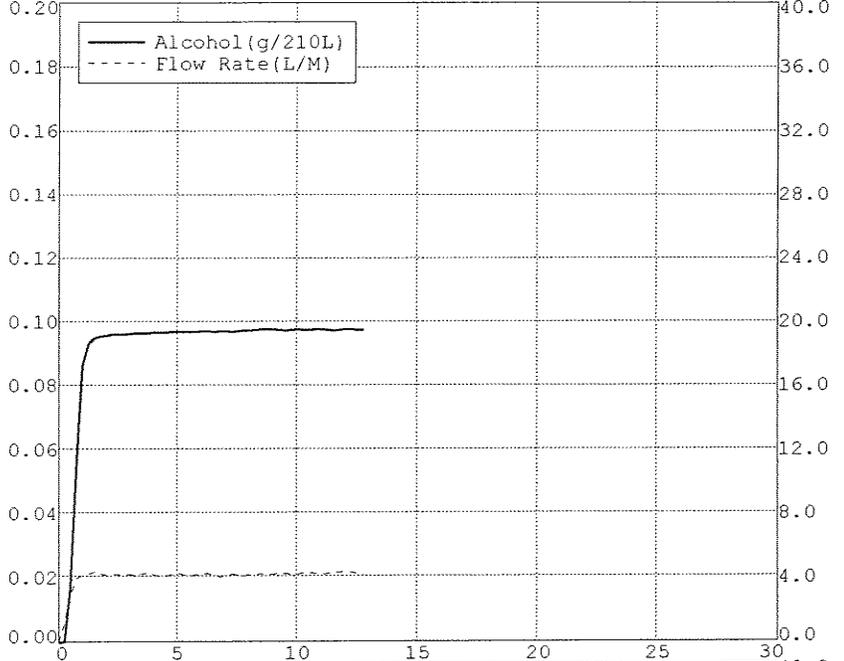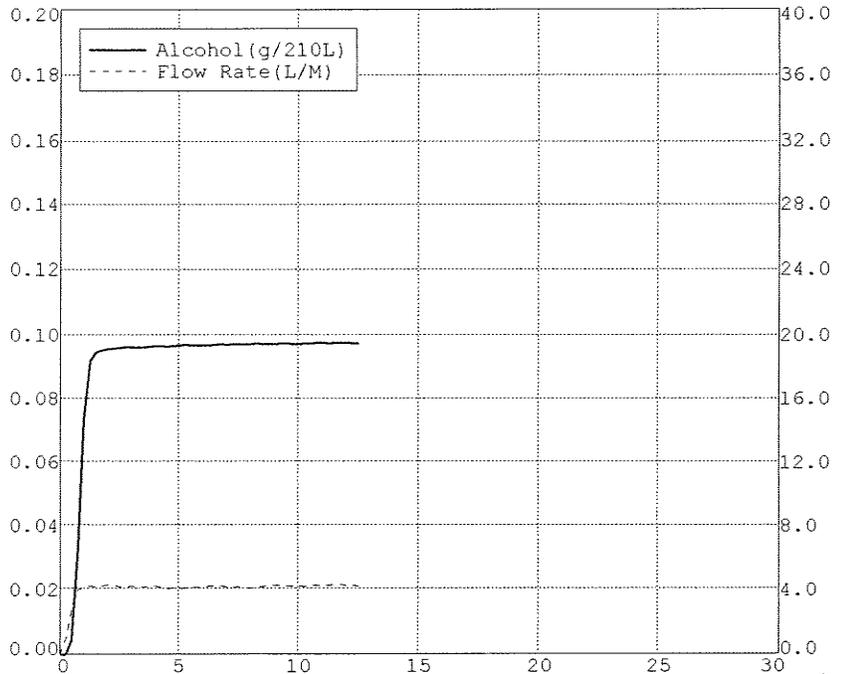

*Sus R/J Bartlett weso #16  
08-09-16*