

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 08/15/2016

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:39
INTERNAL STANDARD	VERIFIED	16:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:41
BLANK TEST	0.00	16:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:42
BLANK TEST	0.00	16:43

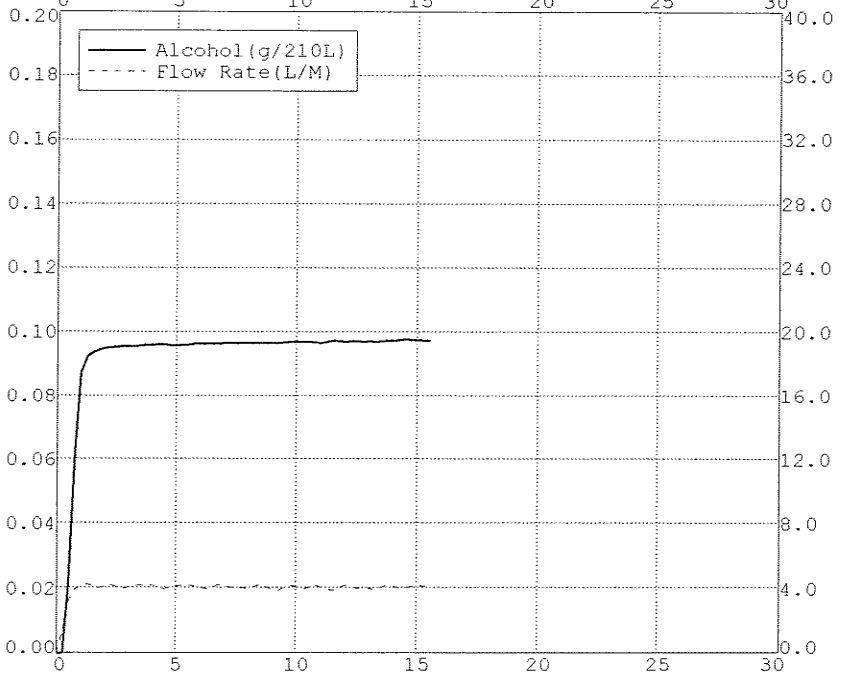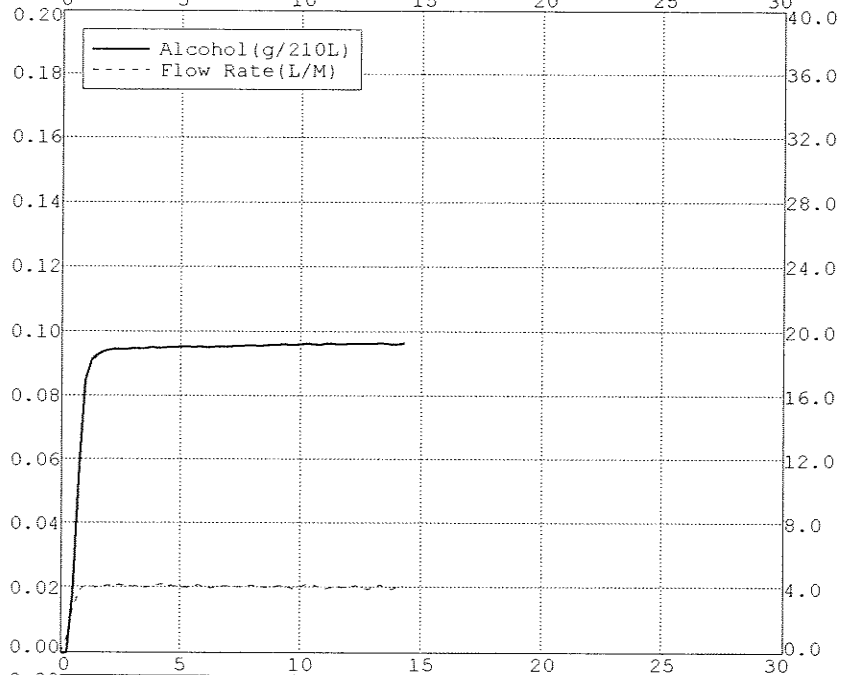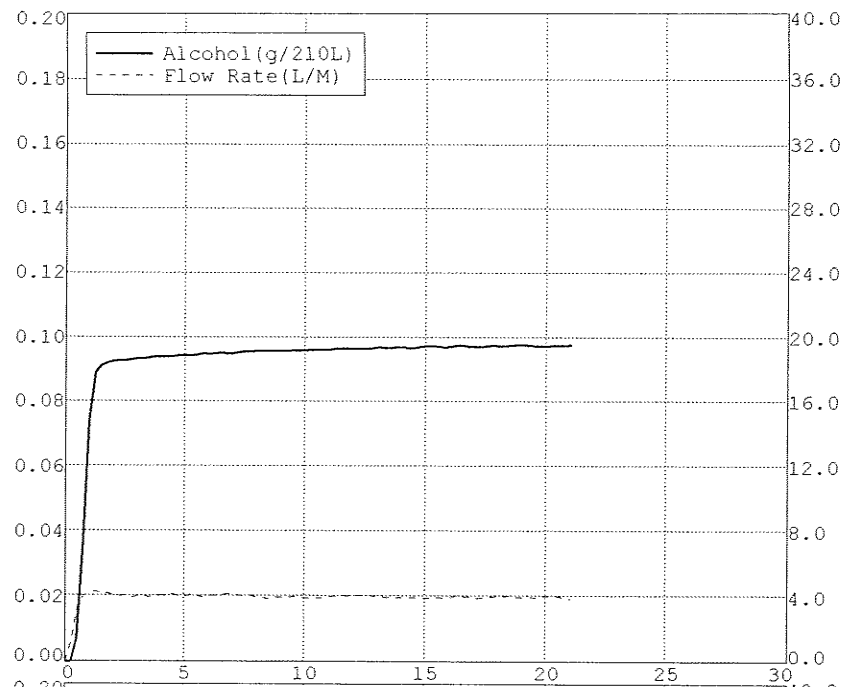

*Charles B. Geisler* #247