

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/15/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:55
INTERNAL STANDARD	VERIFIED	00:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:56
BLANK TEST	0.00	00:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:57
BLANK TEST	0.00	00:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:58
BLANK TEST	0.00	00:59

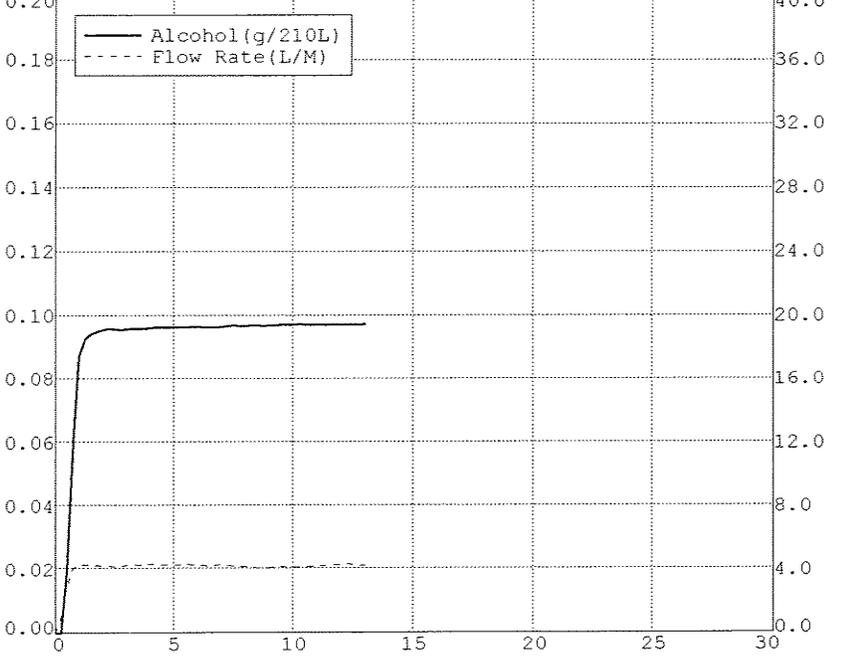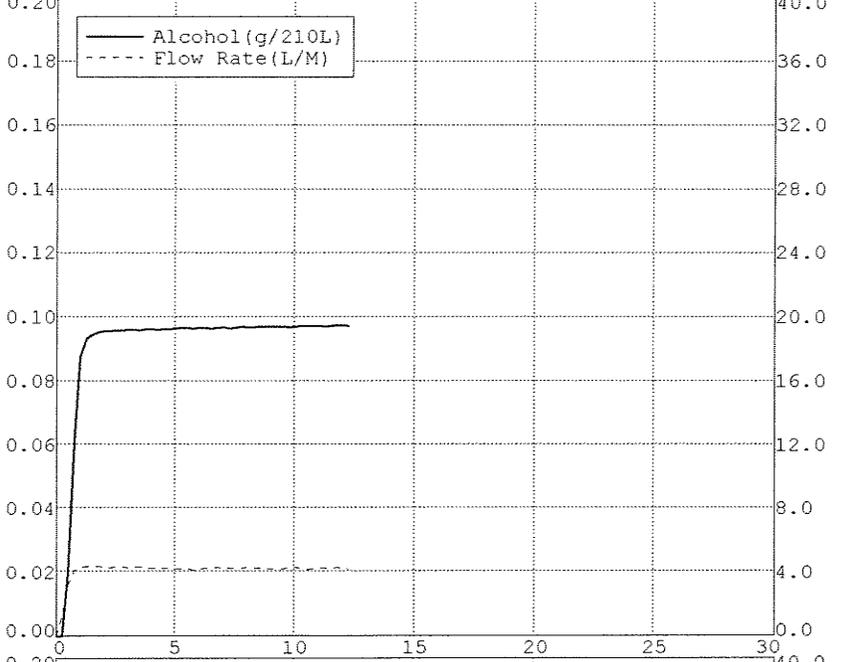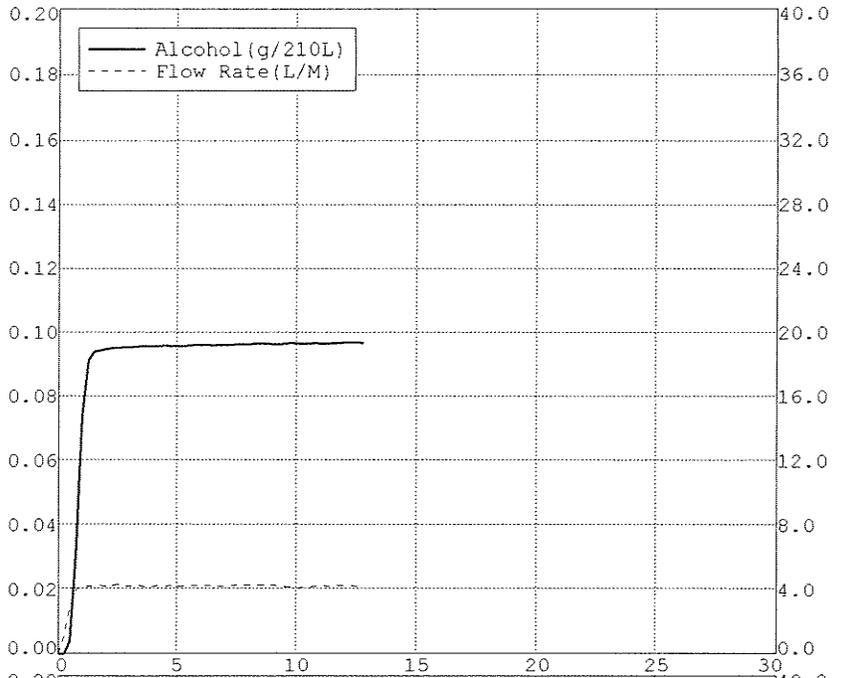

Sgt Ralph Bartlett *Warren #162*
08-15-16