

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/23/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:10
INTERNAL STANDARD	VERIFIED	01:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:10
BLANK TEST	0.00	01:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:11
BLANK TEST	0.00	01:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:13
BLANK TEST	0.00	01:14

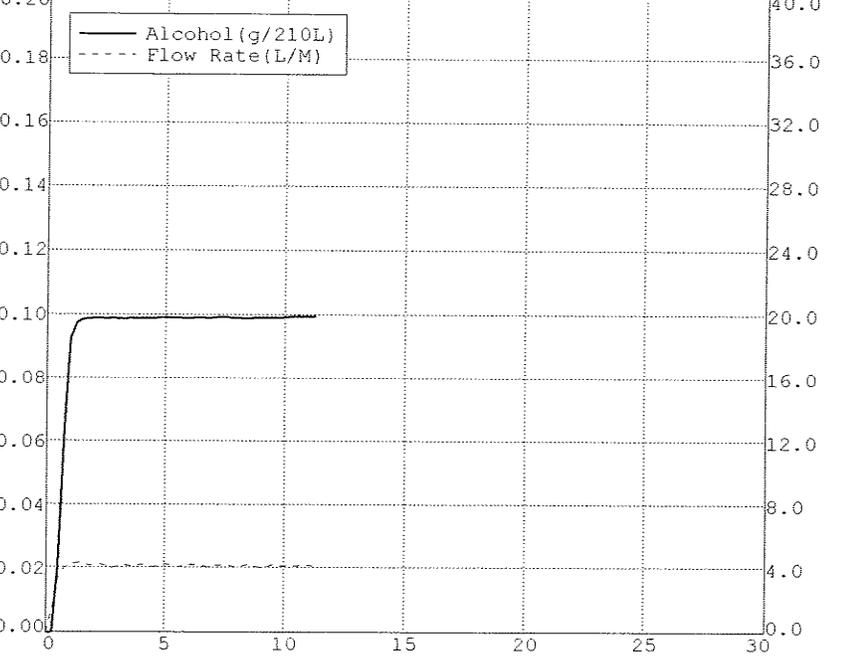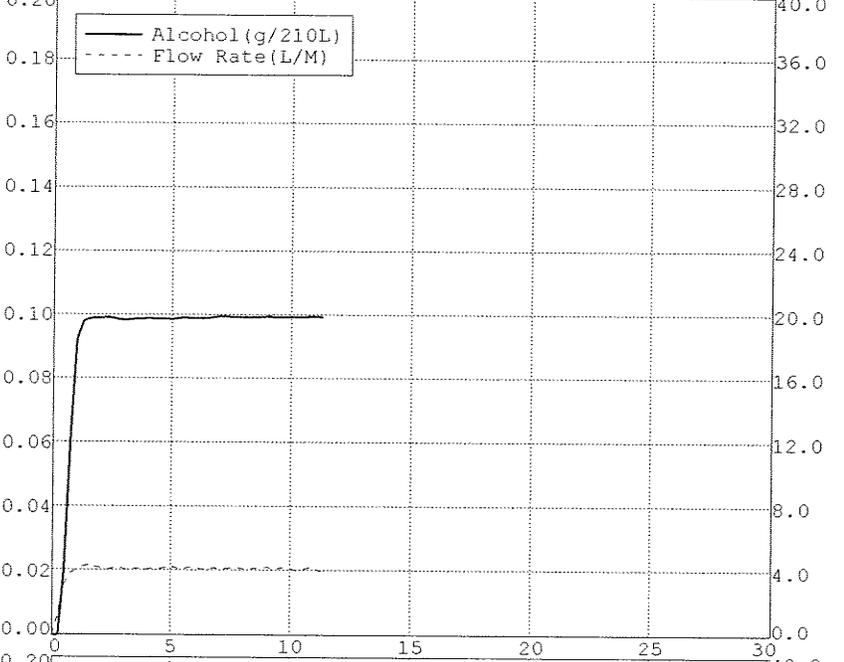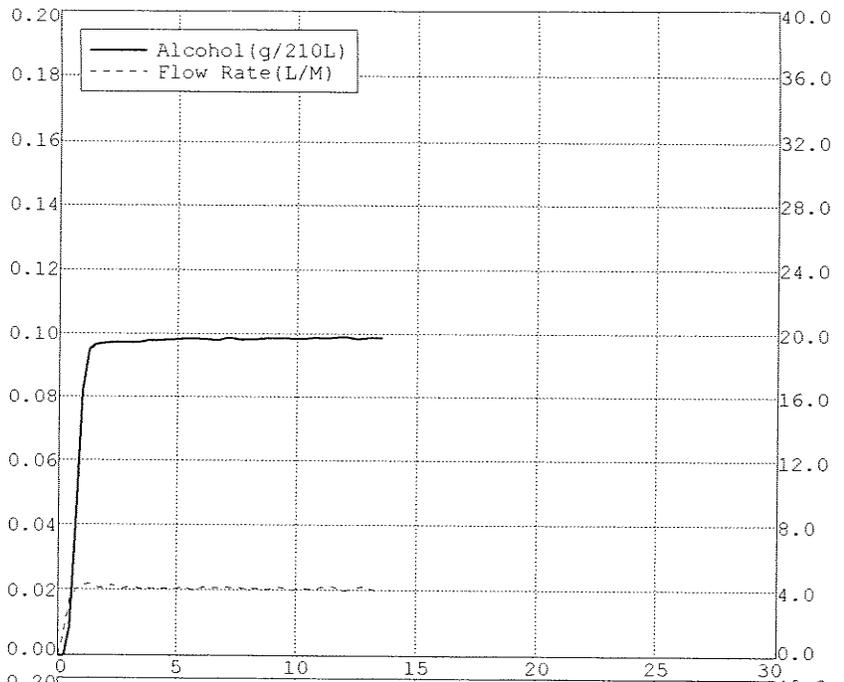

SUS Rpt by Bartlett WCR# 16
08-23-16