

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 09/07/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:38
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:38
BLANK TEST	0.00	00:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	00:41
BLANK TEST	0.00	00:42

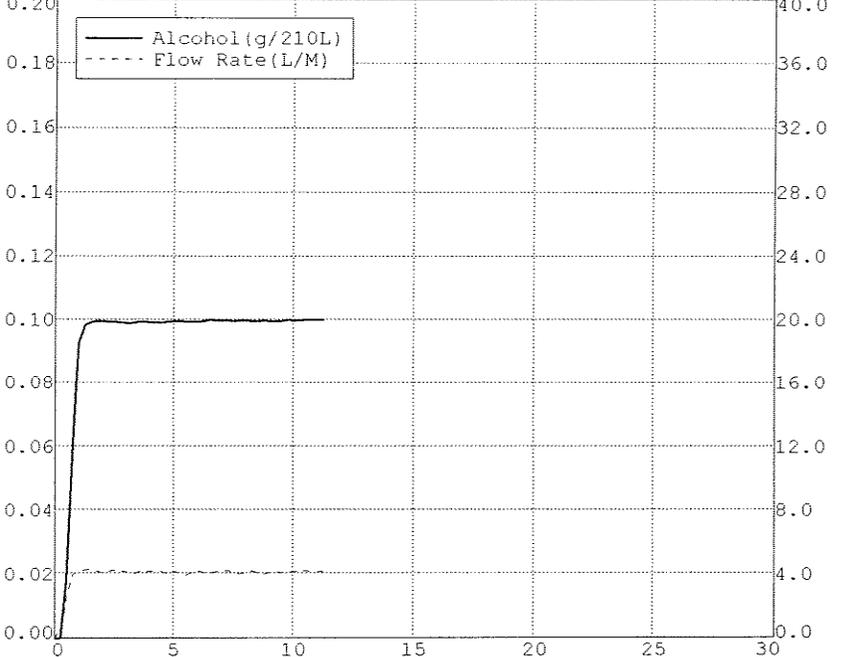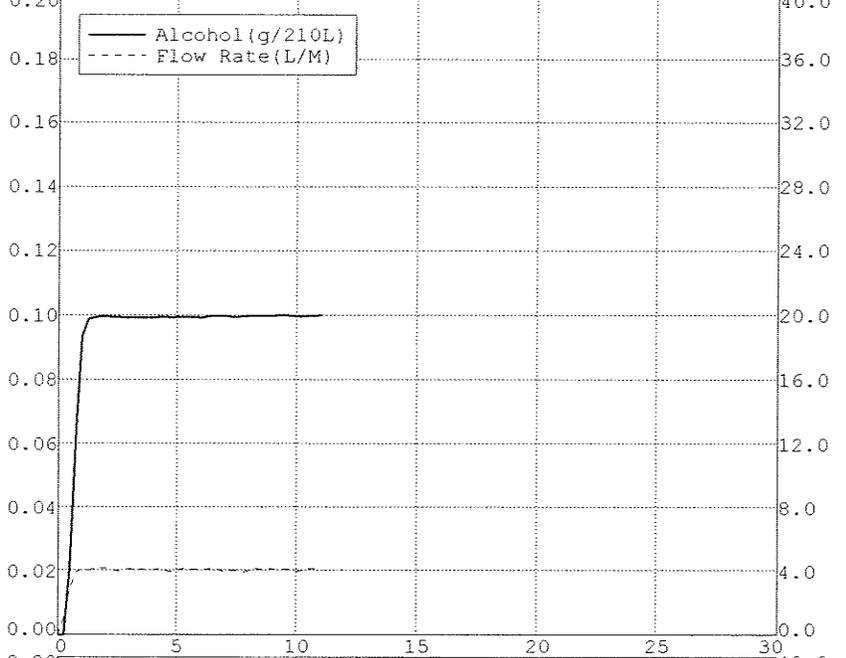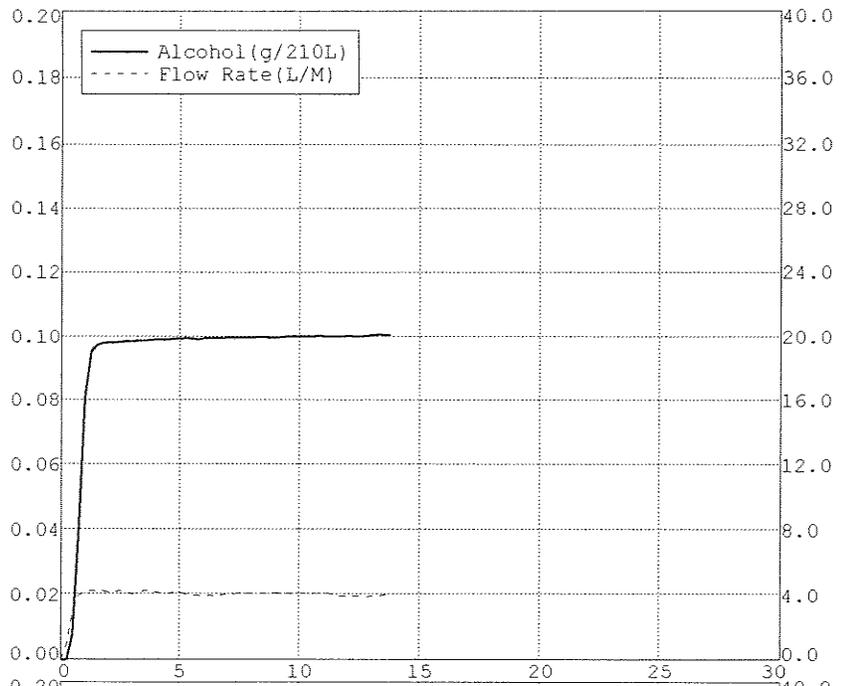

Sgt. R. J. Bartlett
 09-07-16