

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/25/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:20
INTERNAL STANDARD	VERIFIED	20:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:20
BLANK TEST	0.00	20:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:22
BLANK TEST	0.00	20:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:23
BLANK TEST	0.00	20:24

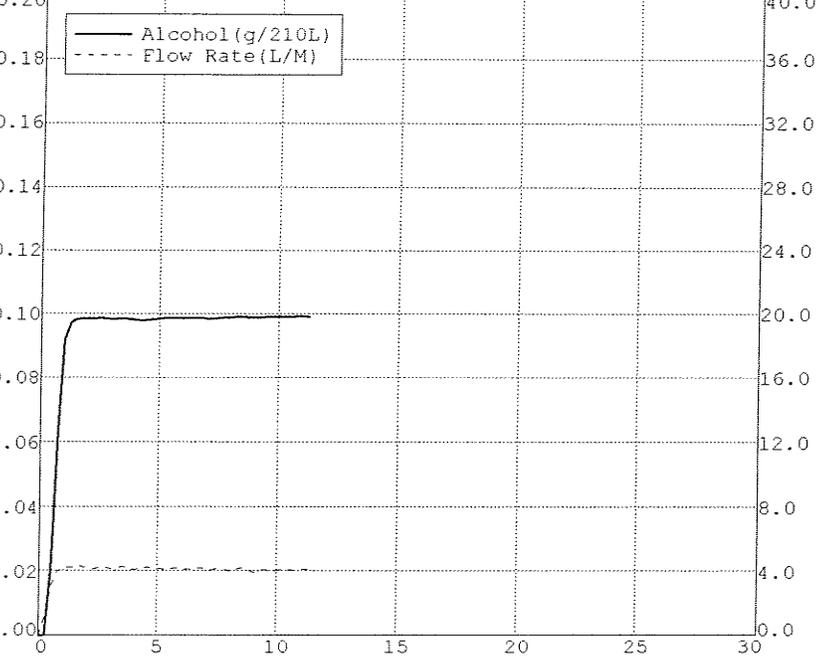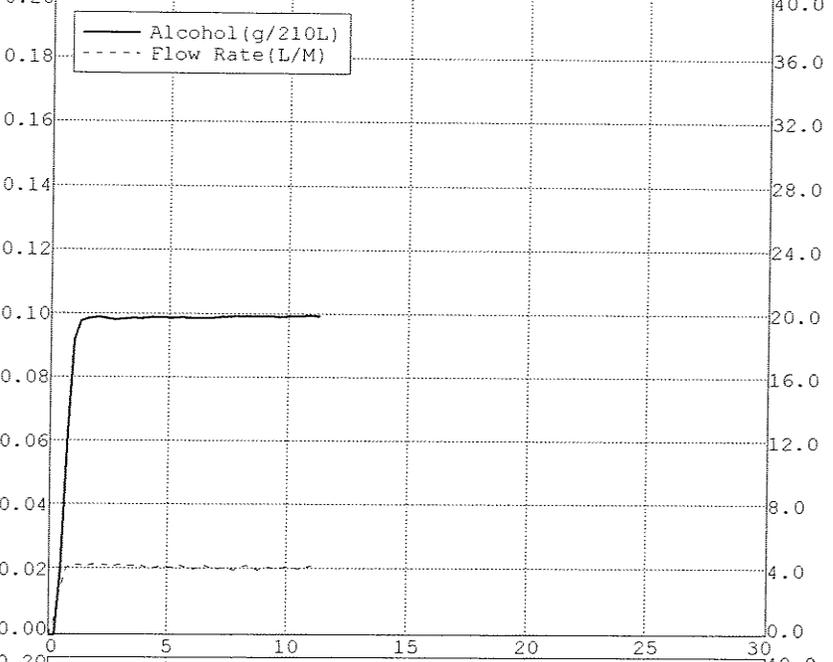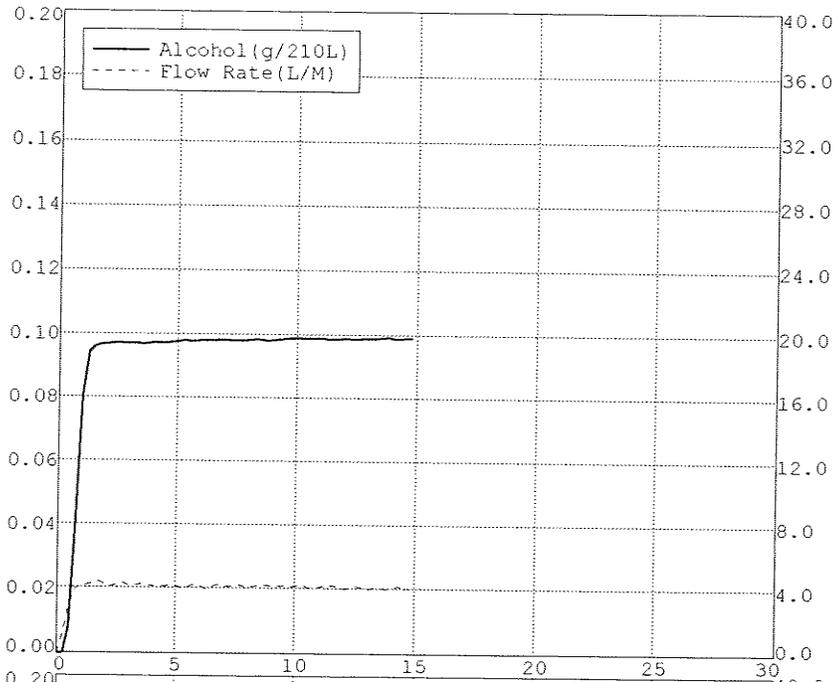

36-7 RJA/Bartlett case #102  
09-25-16