

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 10/02/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:50
INTERNAL STANDARD	VERIFIED	21:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:51
BLANK TEST	0.00	21:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:52
BLANK TEST	0.00	21:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:54
BLANK TEST	0.00	21:55

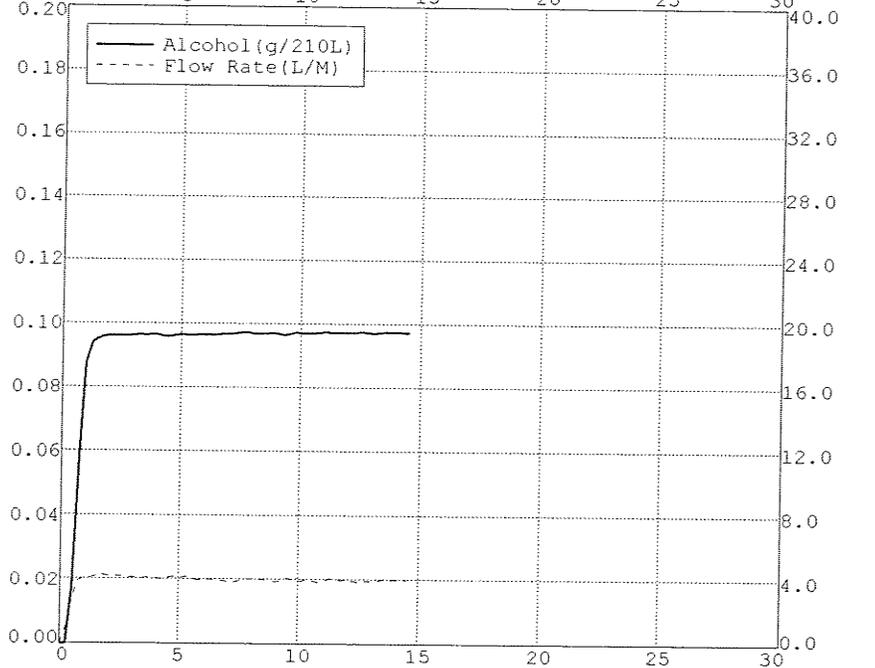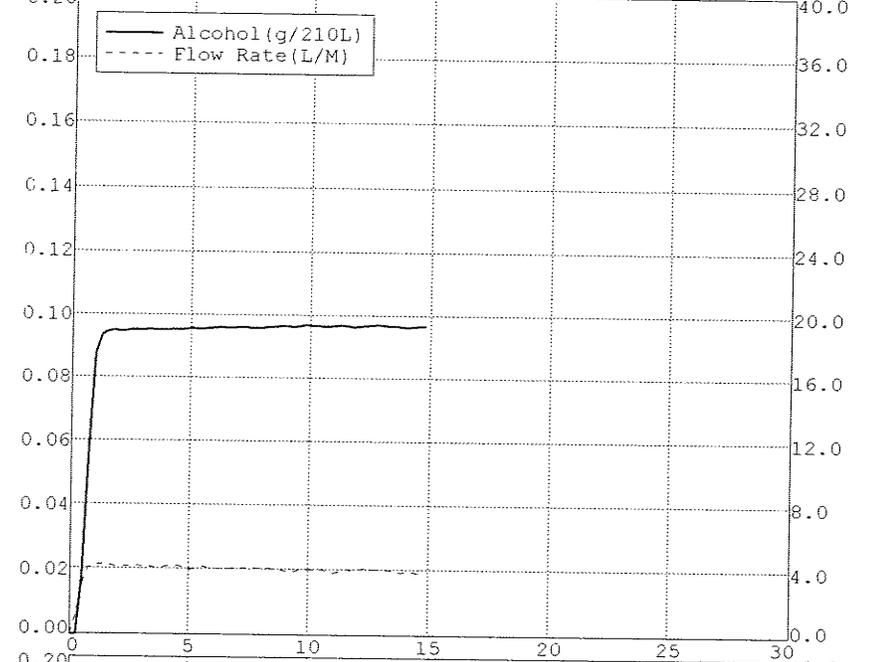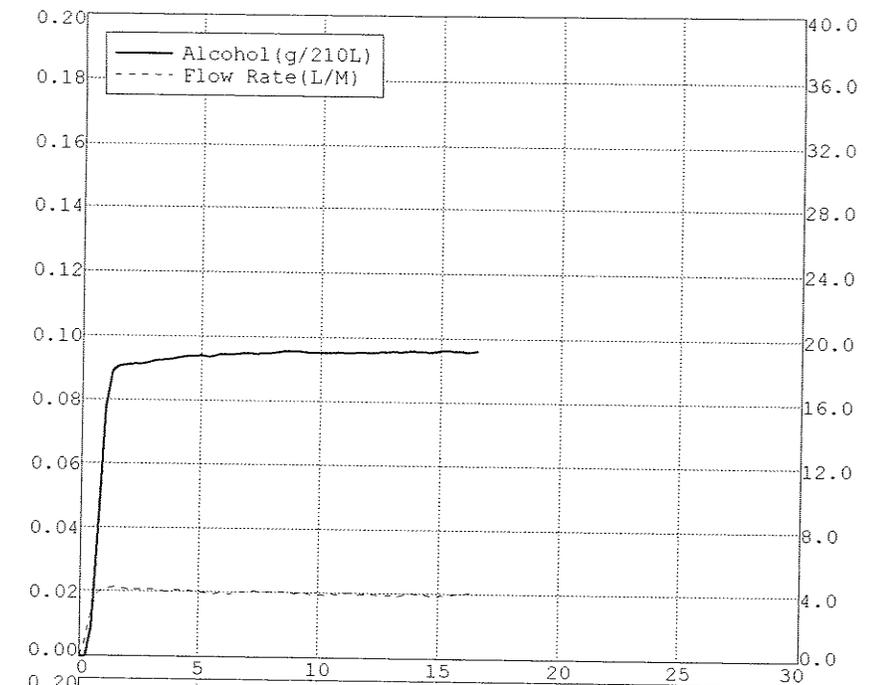

SGS Ralph J Bartlett WOSO #162
 10-02-16