

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 10/24/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:36
INTERNAL STANDARD	VERIFIED	01:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:36
BLANK TEST	0.00	01:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:38
BLANK TEST	0.00	01:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:39
BLANK TEST	0.00	01:40

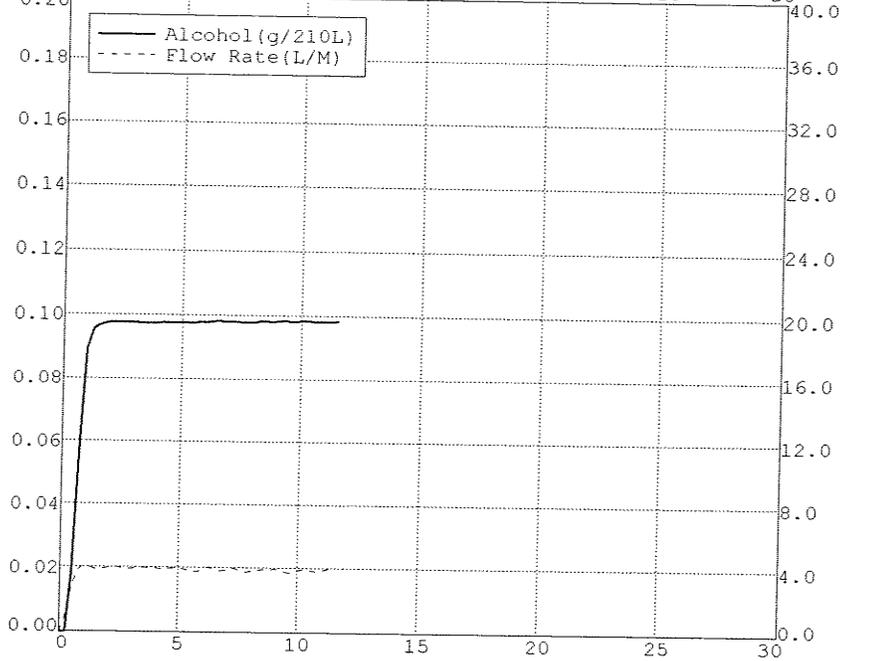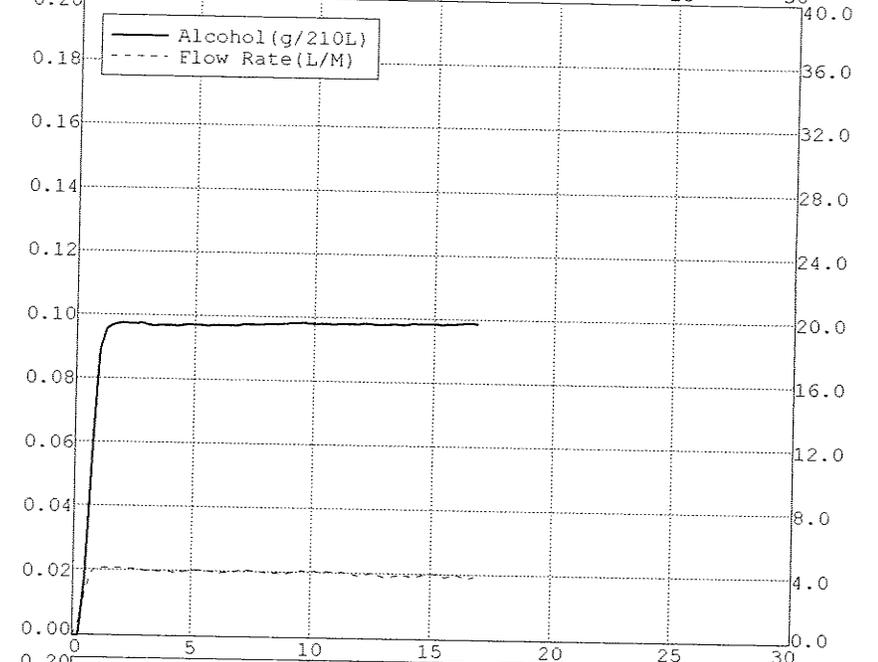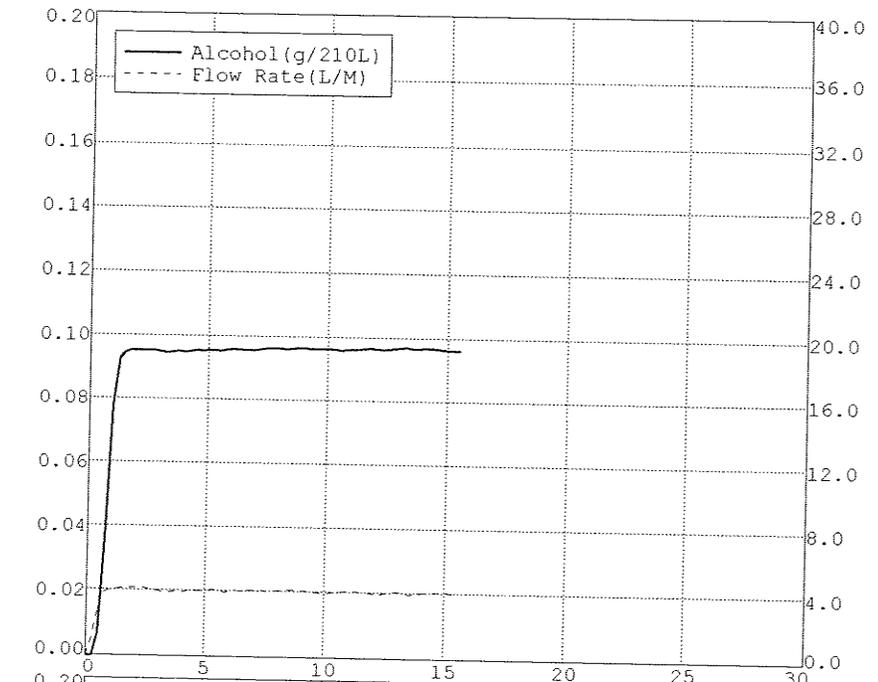

SCS R/J Bartlett WSO #162
10-24-16