

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/07/2016

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:14
INTERNAL STANDARD	VERIFIED	12:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:14
BLANK TEST	0.00	12:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:15
BLANK TEST	0.00	12:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:17
BLANK TEST	0.00	12:18

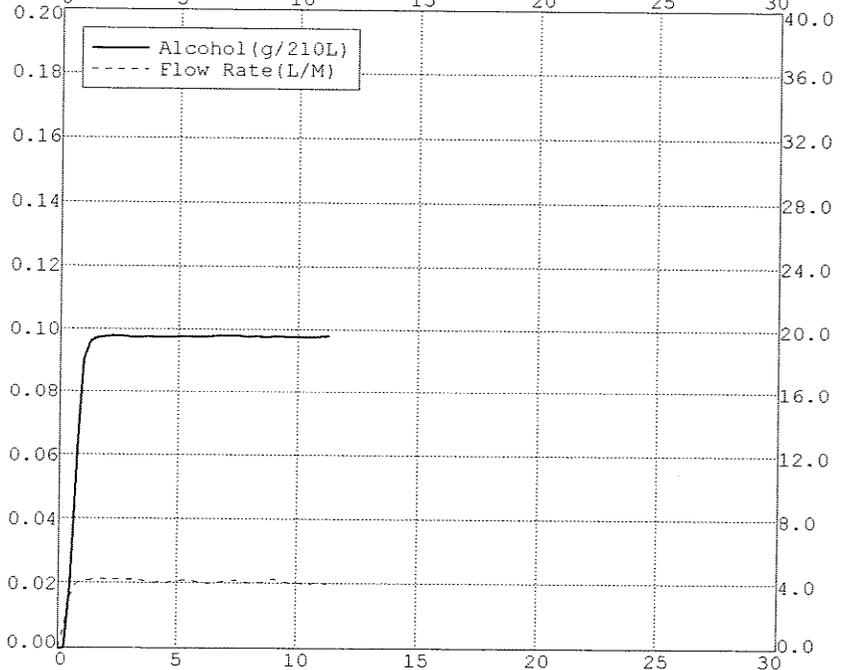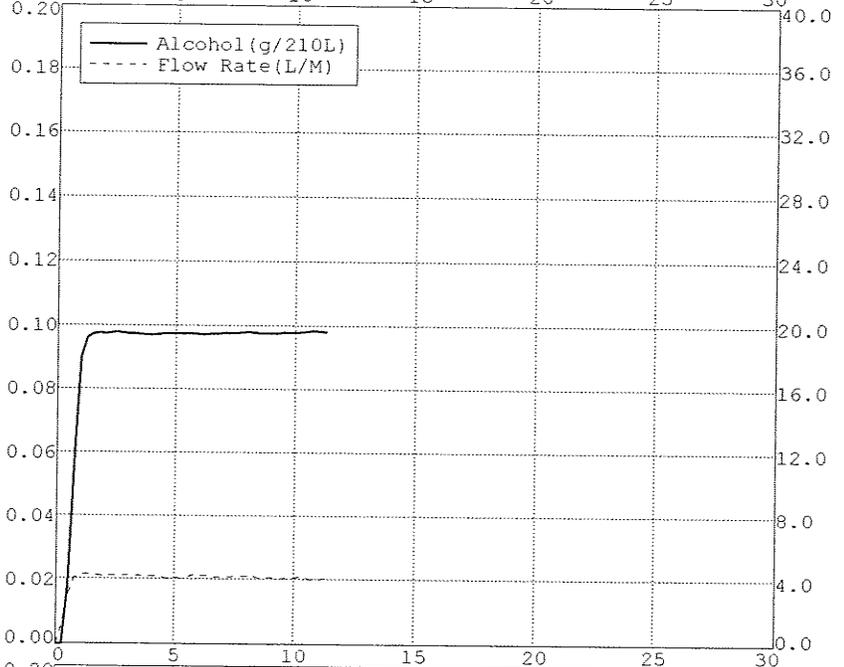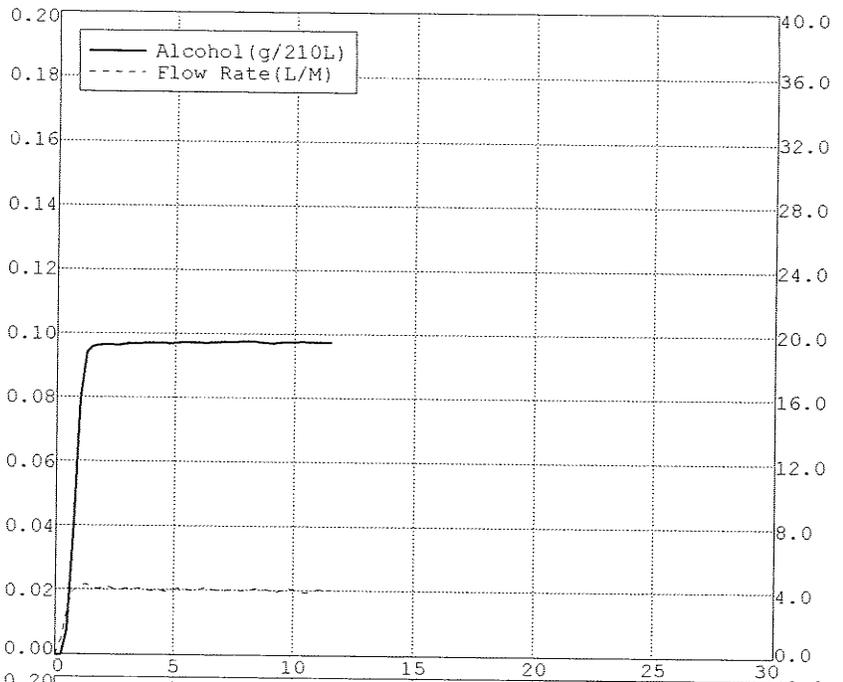

Handwritten signature: A. Charles B. Geisler #245 11/07/16