

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 11/13/2016

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:55
INTERNAL STANDARD	VERIFIED	14:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:55
BLANK TEST	0.00	14:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	14:56
BLANK TEST	0.00	14:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:58
BLANK TEST	0.00	14:59

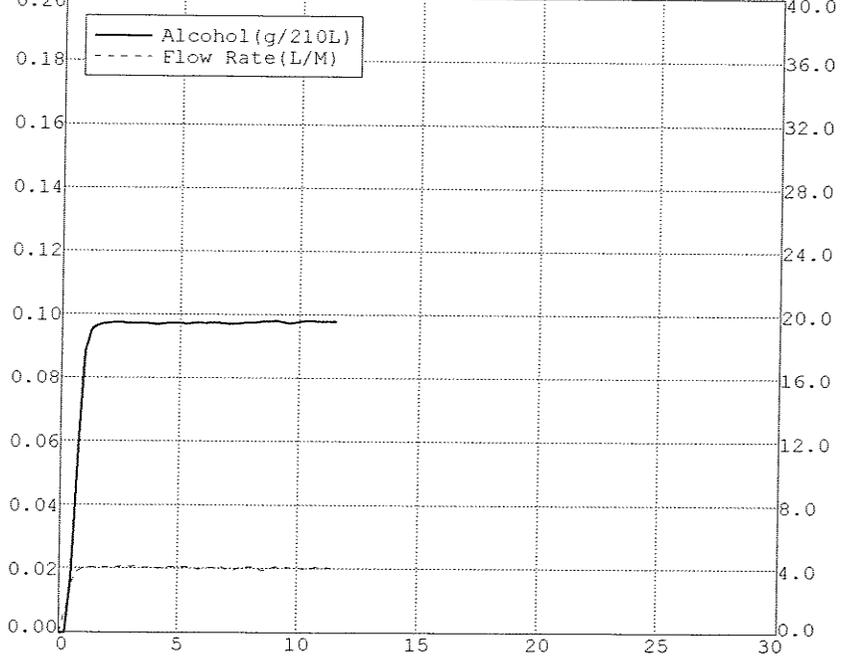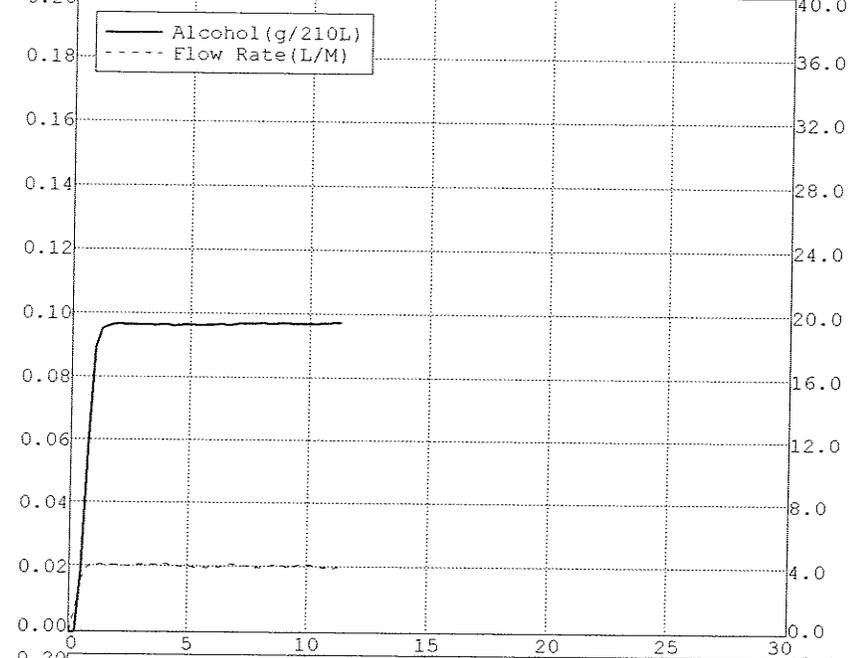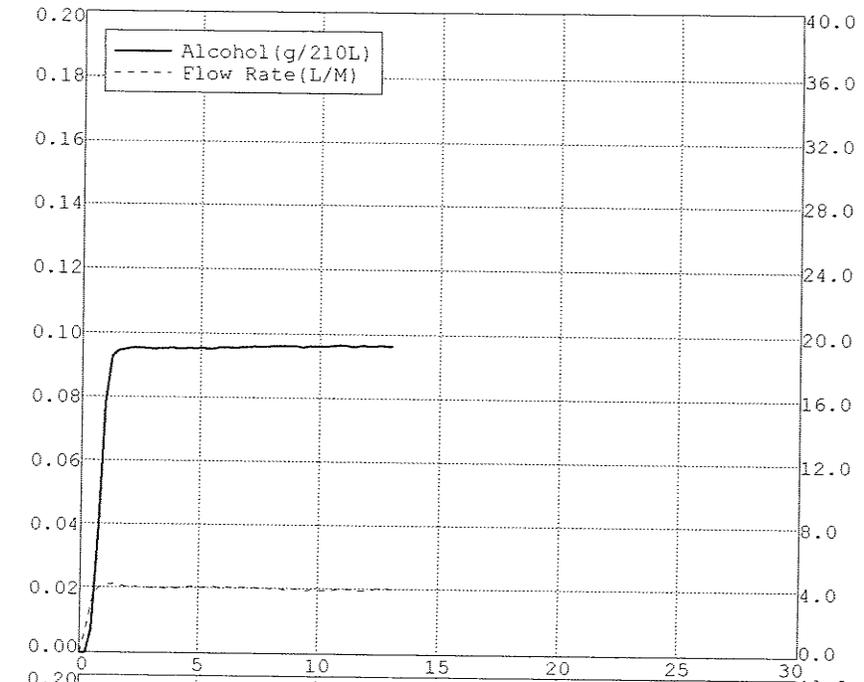

*Handwritten signature: C. B. Geisler #248*