

SOLUTION CHANGE




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 11/29/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16240

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 01:25 |
| INTERNAL STANDARD | VERIFIED | 01:25 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 01:25 |
| BLANK TEST | 0.00 | 01:26 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 01:27 |
| BLANK TEST | 0.00 | 01:28 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 01:28 |
| BLANK TEST | 0.00 | 01:29 |

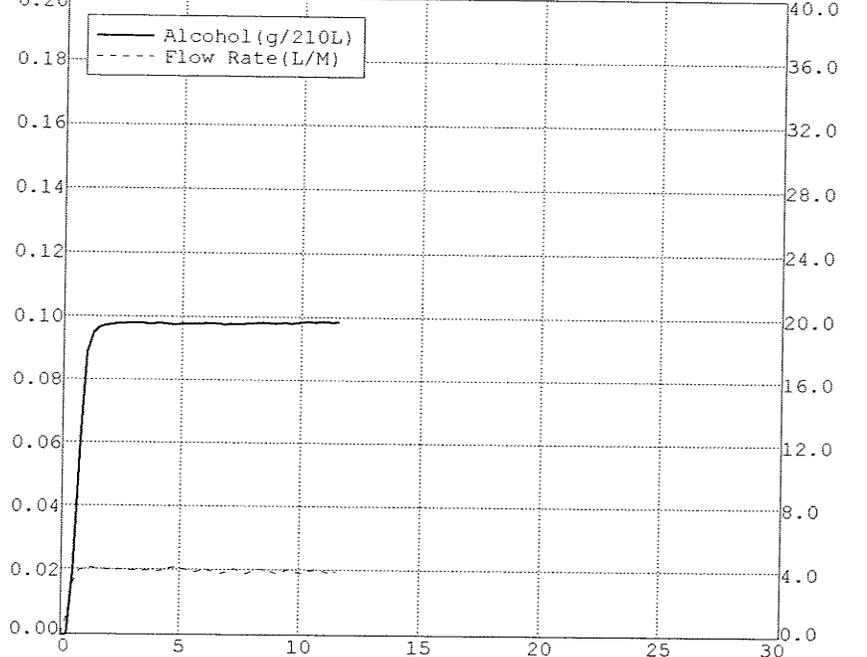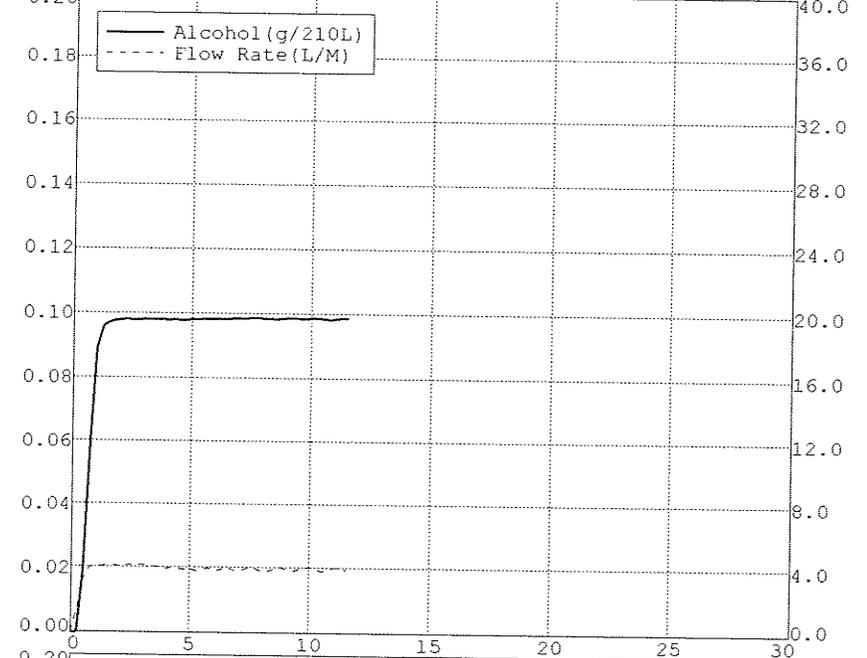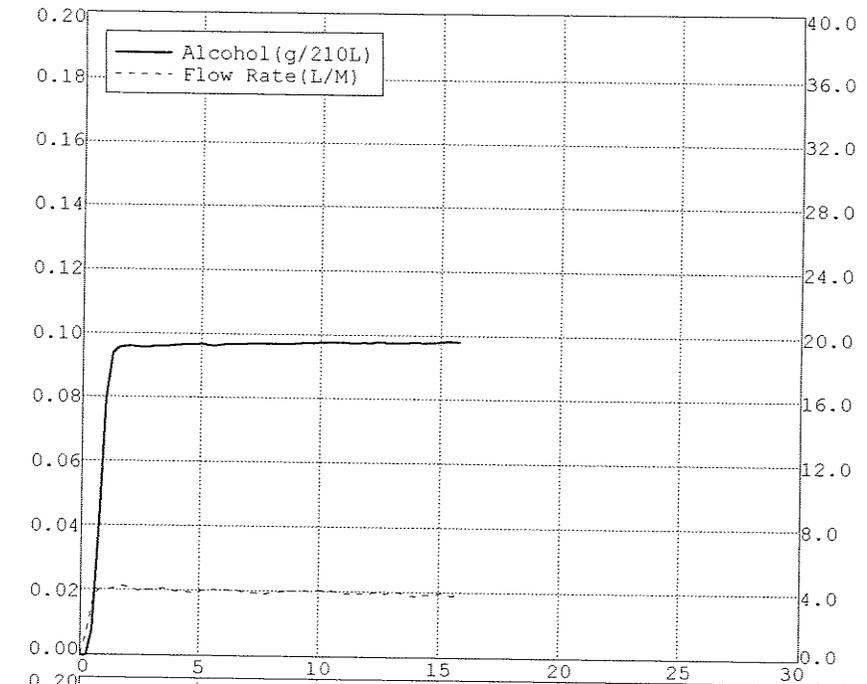

SGT *Ralph Bartlett* weso #162
 11/29/16